




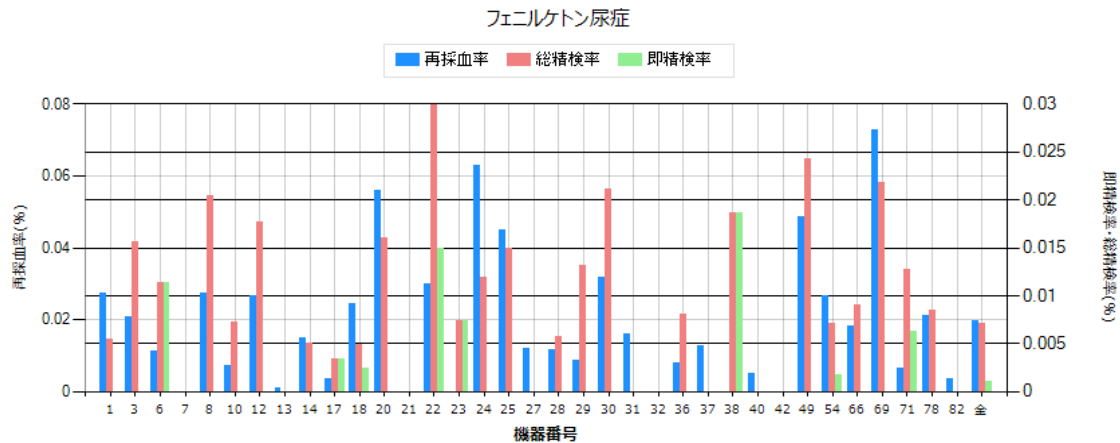


機器No.□	検体数□	再採血数	即精検数	再採血後 精検数	総精検数	発見患者数	再採血率	即精検率	再採血後 精検率	総精検率	発見頻度	陽性適中率 (PPV)
1	54,891	15	0	3	3	2	0.02732	-	0.00546	0.00546	1:27446	66.67
3	19,159	4	0	3	3	3	0.02087	-	0.01565	0.01565	1:6386	100
6	8,759	1	1	0	1	1	0.01141	0.01141	-	0.01141	1:8759	100
7	11,652	0	0	0	0	0	-	-	-	-	-	-
8	14,660	4	0	3	3	1	0.02728	-	0.02046	0.02046	1:14660	33.33
10	13,710	1	0	1	1	1	0.00729	-	0.00729	0.00729	1:13710	100
12	11,270	3	0	2	2	0	0.02661	-	0.01774	0.01774	-	0
13	89,550	1	0	0	0	-	0.00111	-	-	-	-	-
14	39,815	6	0	2	2	1	0.01506	-	0.00502	0.00502	1:39815	50
17	58,597	2	2	0	2	-	0.00341	0.00341	-	0.00341	-	-
18	41,136	10	1	1	2	1	0.0243	0.00243	0.00243	0.00486	1:41136	50
20	12,480	7	0	2	2	2	0.05608	-	0.01602	0.01602	1:6240	100
21	10,798	0	0	0	0	-	-	-	-	-	-	-
22	6,680	2	1	1	2	1	0.02994	0.01497	0.01497	0.02994	1:6680	50
23	13,548	0	1	0	1	1	-	0.00738	-	0.00738	1:13548	100
24	66,779	42	0	8	8	-	0.06289	-	0.01197	0.01197	-	-
25	6,683	3	0	1	1	-	0.04489	-	0.01496	0.01496	-	-
27	8,444	1	0	0	0	0	0.01184	-	-	-	-	-
28	17,318	2	0	1	1	1	0.01154	-	0.00577	0.00577	1:17318	100
29	22,886	2	0	3	3	1	0.00873	-	0.0131	0.0131	1:22886	33.33
30	9,489	3	0	2	2	-	0.03161	-	0.02107	0.02107	-	-
31	24,766	4	0	0	0	0	0.01615	-	-	-	-	-
32	4,702	0	0	0	0	0	-	-	-	-	-	-
36	12,425	1	0	1	1	0	0.00804	-	0.00804	0.00804	-	0
37	7,905	1	0	0	0	-	0.01265	-	-	-	-	-
38	5,357	0	1	0	1	1	-	0.01866	-	0.01866	1:5357	100
40	38,816	2	0	0	0	-	0.00515	-	-	-	-	-
42	6,204	0	0	0	0	0	-	-	-	-	-	-
49	12,337	6	0	3	3	0	0.04863	-	0.02431	0.02431	-	0
54	56,321	15	1	3	4	0	0.02663	0.00177	0.00532	0.0071	-	0
66	22,049	4	0	2	2	0	0.01814	-	0.00907	0.00907	-	0
69	13,731	10	0	3	3	0	0.07282	-	0.02184	0.02184	-	0
71	15,754	1	1	1	2	1	0.00634	0.00634	0.00634	0.01269	1:15754	50
78	47,033	10	0	4	4	2	0.02126	-	0.0085	0.0085	1:23517	50
82	27,685	1	0	0	0	0	0.00361	-	-	-	-	-
全体	833,389	164	9	50	59	20	0.01967	0.00107	0.00599	0.00707	1:41669	33.9
						max	0.07282	0.01866	0.02431	0.02994		100
						min	0.00111	0.00177	0.00243	0.00341		0

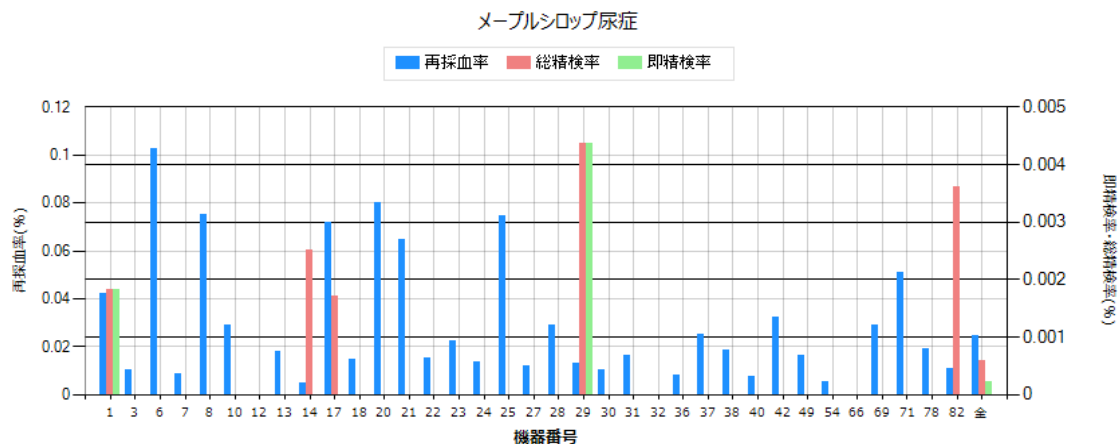


機器No.□	検体数□	再採血数	即精検数	再採血後 精検数	総精検数	発見患者数	再採血率	即精検率	再採血後 精検率	総精検率	発見頻度	陽性適中率 (PPV)
1	54,891	23	1	0	1	0	0.0419	0.00182	-	0.00182	-	0
3	19,159	2	0	0	0	0	0.01043	-	-	-	-	-
6	8,759	9	0	0	0	-	0.10275	-	-	-	-	-
7	11,652	1	0	0	0	0	0.00858	-	-	-	-	-
8	14,660	11	0	0	0	0	0.07503	-	-	-	-	-
10	13,710	4	0	0	0	-	0.02917	-	-	-	-	-
12	11,270	0	0	0	0	0	-	-	-	-	-	-
13	89,550	16	0	0	0	-	0.01786	-	-	-	-	-
14	39,815	2	0	1	1	0	0.00502	-	0.00251	0.00251	-	0
17	58,597	42	0	1	1	-	0.07167	-	0.0017	0.0017	-	-
18	41,136	6	0	0	0	-	0.01458	-	-	-	-	-
20	12,480	10	0	0	0	0	0.08012	-	-	-	-	-
21	10,798	7	0	0	0	-	0.06482	-	-	-	-	-
22	6,680	1	0	0	0	-	0.01497	-	-	-	-	-
23	13,548	3	0	0	0	0	0.02214	-	-	-	-	-
24	66,779	9	0	0	0	-	0.01347	-	-	-	-	-
25	6,683	5	0	0	0	-	0.07481	-	-	-	-	-
27	8,444	1	0	0	0	0	0.01184	-	-	-	-	-
28	17,318	5	0	0	0	0	0.02887	-	-	-	-	-
29	22,886	3	1	0	1	0	0.0131	0.00436	-	0.00436	-	0
30	9,489	1	0	0	0	-	0.01053	-	-	-	-	-
31	24,766	4	0	0	0	0	0.01615	-	-	-	-	-
32	4,702	0	0	0	0	0	-	-	-	-	-	-
36	12,425	1	0	0	0	-	0.00804	-	-	-	-	-
37	7,905	2	0	0	0	-	0.0253	-	-	-	-	-
38	5,357	1	0	0	0	-	0.01866	-	-	-	-	-
40	38,816	3	0	0	0	-	0.00772	-	-	-	-	-
42	6,204	2	0	0	0	0	0.03223	-	-	-	-	-
49	12,337	2	0	0	0	0	0.01621	-	-	-	-	-
54	56,321	3	0	0	0	0	0.00532	-	-	-	-	-
66	22,049	0	0	0	0	0	-	-	-	-	-	-
69	13,731	4	0	0	0	0	0.02913	-	-	-	-	-
71	15,754	8	0	0	0	0	0.05078	-	-	-	-	-
78	47,033	9	0	0	0	-	0.01913	-	-	-	-	-
82	27,685	3	0	1	1	0	0.01083	-	0.00361	0.00361	-	0
全体	833,389	203	2	3	5	0	0.02435	0.00023	0.00035	0.00059	-	0
						max	0.10275	0.00436	0.00361	0.00436		0
						min	0.00502	0.00182	0.0017	0.0017		0

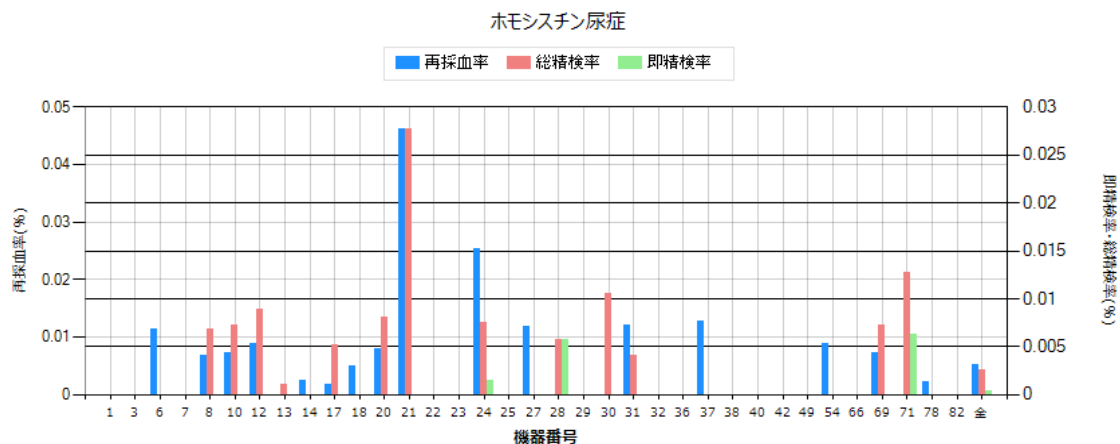


機器No.□	検体数□	再採血数	即精検数	再採血後 精検数	総精検数	発見患者数	再採血率	即精検率	再採血後 精検率	総精検率	発見頻度	陽性適中率 (PPV)
1	54,891	0	0	0	0	0	-	-	-	-	-	-
3	19,159	0	0	0	0	0	-	-	-	-	-	-
6	8,759	1	0	0	0	-	0.01141	-	-	-	-	-
7	11,652	0	0	0	0	0	-	-	-	-	-	-
8	14,660	1	0	1	1	1	0.00682	-	0.00682	0.00682	1:14660	100
10	13,710	1	0	1	1	1	0.00729	-	0.00729	0.00729	1:13710	100
12	11,270	1	0	1	1	0	0.00887	-	0.00887	0.00887	-	0
13	89,550	0	0	0	1	-	-	-	0.00111	0.00111	-	-
14	39,815	1	0	0	0	0	0.00251	-	-	-	-	-
17	58,597	1	0	3	3	-	0.0017	-	0.00511	0.00511	-	-
18	41,136	2	0	0	0	-	0.00486	-	-	-	-	-
20	12,480	1	0	1	1	0	0.00801	-	0.00801	0.00801	-	0
21	10,798	5	0	3	3	-	0.0463	-	0.02778	0.02778	-	-
22	6,680	0	0	0	0	-	-	-	-	-	-	-
23	13,548	0	0	0	0	0	-	-	-	-	-	-
24	66,779	17	1	4	5	-	0.02545	0.00149	0.00598	0.00748	-	-
25	6,683	0	0	0	0	-	-	-	-	-	-	-
27	8,444	1	0	0	0	0	0.01184	-	-	-	-	-
28	17,318	0	1	0	1	0	-	0.00577	-	0.00577	-	0
29	22,886	0	0	0	0	0	-	-	-	-	-	-
30	9,489	0	0	1	1	-	-	-	0.01053	0.01053	-	-
31	24,766	3	0	1	1	1	0.01211	-	0.00403	0.00403	1:24766	100
32	4,702	0	0	0	0	0	-	-	-	-	-	-
36	12,425	0	0	0	0	-	-	-	-	-	-	-
37	7,905	1	0	0	0	-	0.01265	-	-	-	-	-
38	5,357	0	0	0	0	-	-	-	-	-	-	-
40	38,816	0	0	0	0	-	-	-	-	-	-	-
42	6,204	0	0	0	0	0	-	-	-	-	-	-
49	12,337	0	0	0	0	-	-	-	-	-	-	-
54	56,321	5	0	0	0	0	0.00887	-	-	-	-	-
66	22,049	0	0	0	0	0	-	-	-	-	-	-
69	13,731	1	0	1	1	0	0.00728	-	0.00728	0.00728	-	0
71	15,754	0	1	1	2	-	-	0.00634	0.00634	0.01269	-	-
78	47,033	1	0	0	0	-	0.00212	-	-	-	-	-
82	27,685	0	0	0	0	0	-	-	-	-	-	-
全体	833,389	43	3	19	22	3	0.00515	0.00035	0.00227	0.00263	1:277796	13.64
						max	0.0463	0.00634	0.02778	0.02778		100
						min	0.0017	0.00149	0.00111	0.00111		0

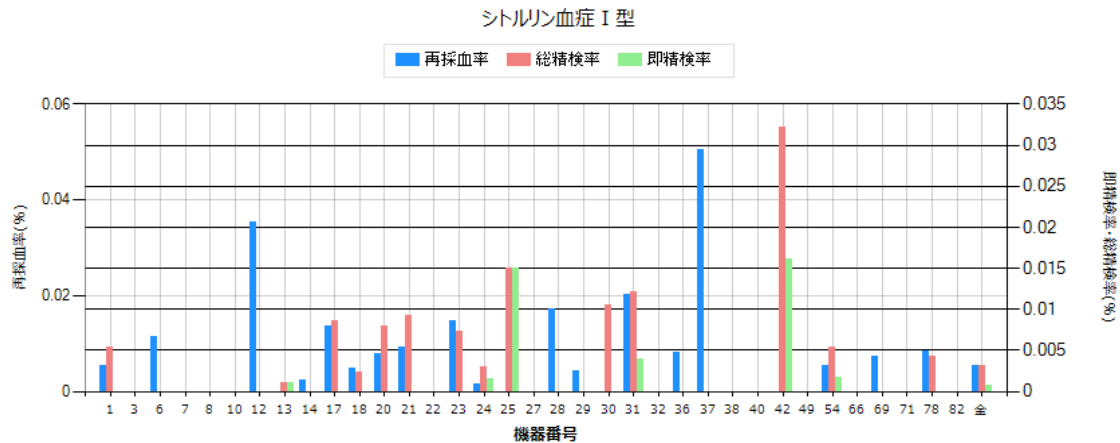


機器No.□	検体数□	再採血数	即精検数	再採血後 精検数	総精検数	発見患者数	再採血率	即精検率	再採血後 精検率	総精検率	発見頻度	陽性適中率 (PPV)
1	54,891	3	0	3	3	0	0.00546	-	0.00546	0.00546	-	0
3	19,159	0	0	0	0	0	-	-	-	-	-	-
6	8,759	1	0	0	0	-	0.01141	-	-	-	-	-
7	11,652	0	0	0	0	0	-	-	-	-	-	-
8	14,660	0	0	0	0	0	-	-	-	-	-	-
10	13,710	0	0	0	0	-	-	-	-	-	-	-
12	11,270	4	0	0	0	0	0.03549	-	-	-	-	-
13	89,550	0	1	0	1	-	-	0.00111	-	0.00111	-	-
14	39,815	1	0	0	0	0	0.00251	-	-	-	-	-
17	58,597	8	0	5	5	-	0.01365	-	0.00853	0.00853	-	-
18	41,136	2	0	1	1	-	0.00486	-	0.00243	0.00243	-	-
20	12,480	1	0	1	1	0	0.00801	-	0.00801	0.00801	-	0
21	10,798	1	0	1	1	-	0.00926	-	0.00926	0.00926	-	-
22	6,680	0	0	0	0	-	-	-	-	-	-	-
23	13,548	2	0	1	1	0	0.01476	-	0.00738	0.00738	-	0
24	66,779	1	1	1	2	-	0.00149	0.00149	0.00149	0.00299	-	-
25	6,683	0	1	0	1	1	-	0.01496	-	0.01496	1:6683	100
27	8,444	0	0	0	0	0	-	-	-	-	-	-
28	17,318	3	0	0	0	0	0.01732	-	-	-	-	-
29	22,886	1	0	0	0	0	0.00436	-	-	-	-	-
30	9,489	0	0	1	1	-	-	-	0.01053	0.01053	-	-
31	24,766	5	1	2	3	1	0.02018	0.00403	0.00807	0.01211	1:24766	33.33
32	4,702	0	0	0	0	0	-	-	-	-	-	-
36	12,425	1	0	0	0	-	0.00804	-	-	-	-	-
37	7,905	4	0	0	0	-	0.0506	-	-	-	-	-
38	5,357	0	0	0	0	-	-	-	-	-	-	-
40	38,816	0	0	0	0	-	-	-	-	-	-	-
42	6,204	0	1	1	2	0	-	0.01611	0.01611	0.03223	-	0
49	12,337	0	0	0	0	-	-	-	-	-	-	-
54	56,321	3	1	2	3	0	0.00532	0.00177	0.00355	0.00532	-	0
66	22,049	0	0	0	0	0	-	-	-	-	-	-
69	13,731	1	0	0	0	0	0.00728	-	-	-	-	-
71	15,754	0	0	0	0	0	-	-	-	-	-	-
78	47,033	4	0	2	2	-	0.0085	-	0.00425	0.00425	-	-
82	27,685	0	0	0	0	0	-	-	-	-	-	-
全体	833,389	46	6	21	27	2	0.00551	0.00071	0.00251	0.00323	1:416694	7.41
						max	0.0506	0.01611	0.01611	0.03223		100
						min	0.00149	0.00111	0.00149	0.00111		0

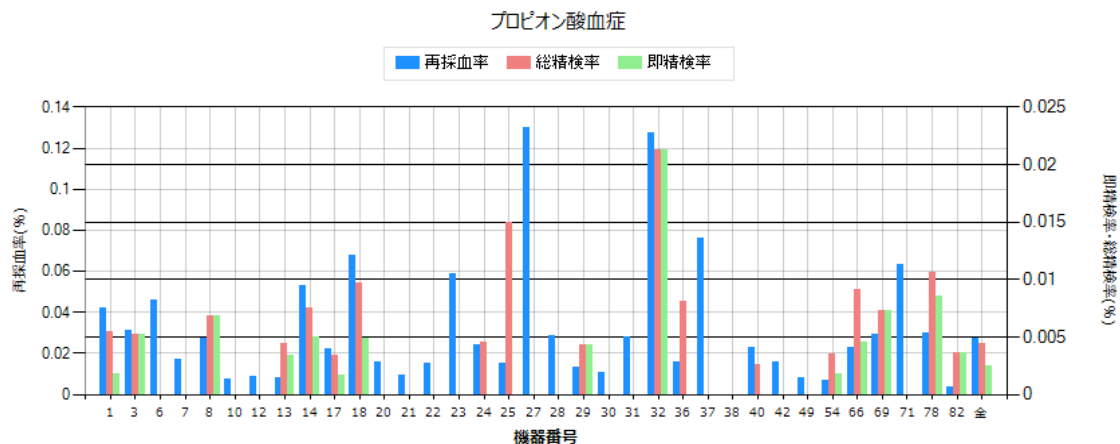


機器No.□	検体数□	再採血数	即精検数	再採血後 精検数	総精検数	発見患者数	再採血率	即精検率	再採血後 精検率	総精検率	発見頻度	陽性適中率 (PPV)
1	54,891	23	1	2	3	2	0.0419	0.00182	0.00364	0.00546	1:27446	66.67
3	19,159	6	1	0	1	0	0.03131	0.00521	-	0.00521	-	0
6	8,759	4	0	0	0	-	0.04566	-	-	-	-	-
7	11,652	2	0	0	0	0	0.01716	-	-	-	-	-
8	14,660	4	1	0	1	0	0.02728	0.00682	-	0.00682	-	0
10	13,710	1	0	0	0	-	0.00729	-	-	-	-	-
12	11,270	1	0	0	0	0	0.00887	-	-	-	-	-
13	89,550	7	3	1	4	2	0.00781	0.00335	0.00111	0.00446	1:44775	50
14	39,815	21	2	1	3	0	0.05274	0.00502	0.00251	0.00753	-	0
17	58,597	13	1	1	2	-	0.02218	0.0017	0.0017	0.00341	-	-
18	41,136	28	2	2	4	1	0.06806	0.00486	0.00486	0.00972	1:41136	25
20	12,480	2	0	0	0	0	0.01602	-	-	-	-	-
21	10,798	1	0	0	0	-	0.00926	-	-	-	-	-
22	6,680	1	0	0	0	-	0.01497	-	-	-	-	-
23	13,548	8	0	0	0	0	0.05904	-	-	-	-	-
24	66,779	16	0	3	3	-	0.02395	-	0.00449	0.00449	-	-
25	6,683	1	0	1	1	1	0.01496	-	0.01496	0.01496	1:6683	100
27	8,444	11	0	0	0	0	0.13027	-	-	-	-	-
28	17,318	5	0	0	0	0	0.02887	-	-	-	-	-
29	22,886	3	1	0	1	1	0.0131	0.00436	-	0.00436	1:22886	100
30	9,489	1	0	0	0	-	0.01053	-	-	-	-	-
31	24,766	7	0	0	0	0	0.02826	-	-	-	-	-
32	4,702	6	1	0	1	0	0.1276	0.02126	-	0.02126	-	0
36	12,425	2	0	1	1	0	0.01609	-	0.00804	0.00804	-	0
37	7,905	6	0	0	0	-	0.0759	-	-	-	-	-
38	5,357	0	0	0	0	-	-	-	-	-	-	-
40	38,816	9	0	1	1	-	0.02318	-	0.00257	0.00257	-	-
42	6,204	1	0	0	0	0	0.01611	-	-	-	-	-
49	12,337	1	0	0	0	0	0.0081	-	-	-	-	-
54	56,321	4	1	1	2	1	0.0071	0.00177	0.00177	0.00355	1:56321	50
66	22,049	5	1	1	2	0	0.02267	0.00453	0.00453	0.00907	-	0
69	13,731	4	1	0	1	0	0.02913	0.00728	-	0.00728	-	0
71	15,754	10	0	0	0	0	0.06347	-	-	-	-	-
78	47,033	14	4	1	5	3	0.02976	0.0085	0.00212	0.01063	1:15678	60
82	27,685	1	1	0	1	0	0.00361	0.00361	-	0.00361	-	0
全体	833,389	229	21	16	37	11	0.02747	0.00251	0.00191	0.00443	1:75763	29.73
						max	0.13027	0.02126	0.01496	0.02126		100
						min	0.00361	0.0017	0.00111	0.00257		0

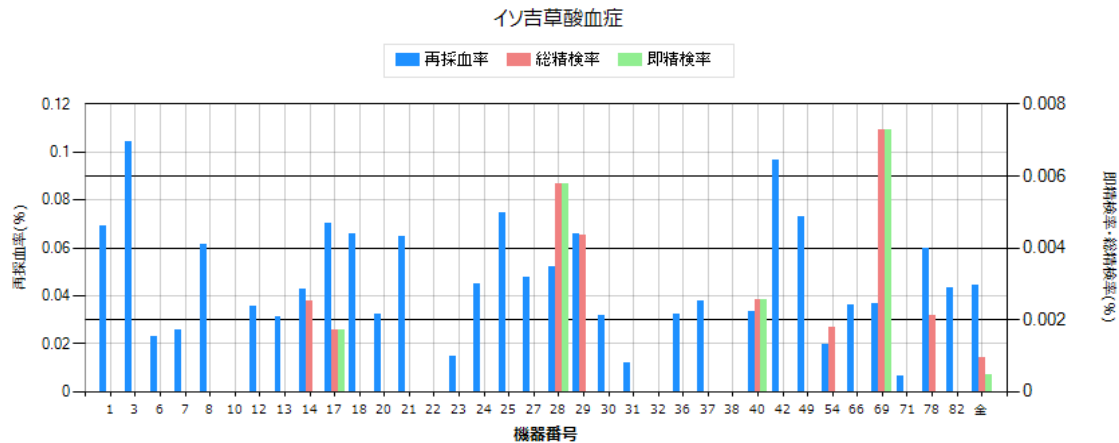


機器No.□	検体数□	再採血数	即精検数	再採血後 精検数	総精検数	発見患者数	再採血率	即精検率	再採血後 精検率	総精検率	発見頻度	陽性適中率 (PPV)
1	54,891	38	0	0	0	0	0.06922	-	-	-	-	-
3	19,159	20	0	0	0	0	0.10438	-	-	-	-	-
6	8,759	2	0	0	0	-	0.02283	-	-	-	-	-
7	11,652	3	0	0	0	0	0.02574	-	-	-	-	-
8	14,660	9	0	0	0	0	0.06139	-	-	-	-	-
10	13,710	0	0	0	0	-	-	-	-	-	-	-
12	11,270	4	0	0	0	0	0.03549	-	-	-	-	-
13	89,550	28	0	0	0	-	0.03126	-	-	-	-	-
14	39,815	17	0	1	1	1	0.04269	-	0.00251	0.00251	1:39815	100
17	58,597	41	1	0	1	-	0.06996	0.0017	-	0.0017	-	-
18	41,136	27	0	0	0	-	0.06563	-	-	-	-	-
20	12,480	4	0	0	0	0	0.03205	-	-	-	-	-
21	10,798	7	0	0	0	-	0.06482	-	-	-	-	-
22	6,680	0	0	0	0	-	-	-	-	-	-	-
23	13,548	2	0	0	0	0	0.01476	-	-	-	-	-
24	66,779	30	0	0	0	-	0.04492	-	-	-	-	-
25	6,683	5	0	0	0	-	0.07481	-	-	-	-	-
27	8,444	4	0	0	0	0	0.04737	-	-	-	-	-
28	17,318	9	1	0	1	0	0.05196	0.00577	-	0.00577	-	0
29	22,886	15	0	1	1	0	0.06554	-	0.00436	0.00436	-	0
30	9,489	3	0	0	0	-	0.03161	-	-	-	-	-
31	24,766	3	0	0	0	0	0.01211	-	-	-	-	-
32	4,702	0	0	0	0	0	-	-	-	-	-	-
36	12,425	4	0	0	0	-	0.03219	-	-	-	-	-
37	7,905	3	0	0	0	-	0.03795	-	-	-	-	-
38	5,357	0	0	0	0	-	-	-	-	-	-	-
40	38,816	13	1	0	1	-	0.03349	0.00257	-	0.00257	-	-
42	6,204	6	0	0	0	0	0.09671	-	-	-	-	-
49	12,337	9	0	0	0	0	0.07295	-	-	-	-	-
54	56,321	11	0	1	1	0	0.01953	-	0.00177	0.00177	-	0
66	22,049	8	0	0	0	0	0.03628	-	-	-	-	-
69	13,731	5	1	0	1	0	0.03641	0.00728	-	0.00728	-	0
71	15,754	1	0	0	0	0	0.00634	-	-	-	-	-
78	47,033	28	0	1	1	-	0.05953	-	0.00212	0.00212	-	-
82	27,685	12	0	0	0	0	0.04334	-	-	-	-	-
全体	833,389	371	4	4	8	1	0.04451	0.00047	0.00047	0.00095	1:833389	12.5
						max	0.10438	0.00728	0.00436	0.00728		100
						min	0.00634	0.0017	0.00177	0.0017		0

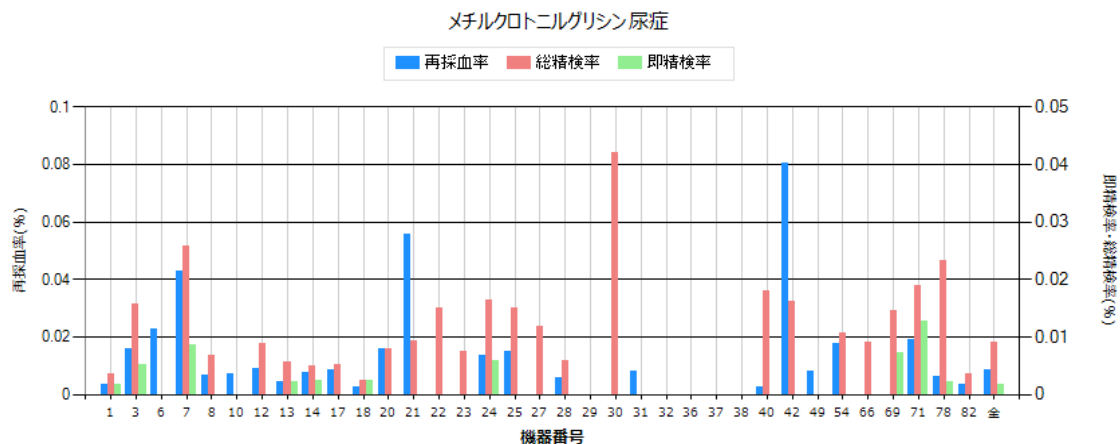


機器No.□	検体数□	再採血数	即精検数	再採血後 精検数	総精検数	発見患者数	再採血率	即精検率	再採血後 精検率	総精検率	発見頻度	陽性適中率 (PPV)
1	54,891	2	1	1	2	0	0.00364	0.00182	0.00182	0.00364	-	0
3	19,159	3	1	2	3	0	0.01565	0.00521	0.01043	0.01565	-	0
6	8,759	2	0	0	0	-	0.02283	-	-	-	-	-
7	11,652	5	1	2	3	1	0.04291	0.00858	0.01716	0.02574	1:11652	33.33
8	14,660	1	0	1	1	0	0.00682	-	0.00682	0.00682	-	0
10	13,710	1	0	0	0	-	0.00729	-	-	-	-	-
12	11,270	1	0	1	1	0	0.00887	-	0.00887	0.00887	-	0
13	89,550	4	2	3	5	2	0.00446	0.00223	0.00335	0.00558	1:44775	40
14	39,815	3	1	1	2	0	0.00753	0.00251	0.00251	0.00502	-	0
17	58,597	5	0	3	3	-	0.00853	-	0.00511	0.00511	-	-
18	41,136	1	1	0	1	-	0.00243	0.00243	-	0.00243	-	-
20	12,480	2	0	1	1	0	0.01602	-	0.00801	0.00801	-	0
21	10,798	6	0	1	1	-	0.05556	-	0.00926	0.00926	-	-
22	6,680	0	0	1	1	0	-	-	0.01497	0.01497	-	0
23	13,548	0	0	1	1	0	-	-	0.00738	0.00738	-	0
24	66,779	9	4	7	11	-	0.01347	0.00598	0.01048	0.01647	-	-
25	6,683	1	0	1	1	-	0.01496	-	0.01496	0.01496	-	-
27	8,444	0	0	1	1	0	-	-	0.01184	0.01184	-	0
28	17,318	1	0	1	1	0	0.00577	-	0.00577	0.00577	-	0
29	22,886	0	0	0	0	0	-	-	-	-	-	-
30	9,489	0	0	4	4	-	-	-	0.04215	0.04215	-	-
31	24,766	2	0	0	0	0	0.00807	-	-	-	-	-
32	4,702	0	0	0	0	0	-	-	-	-	-	-
36	12,425	0	0	0	0	-	-	-	-	-	-	-
37	7,905	0	0	0	0	-	-	-	-	-	-	-
38	5,357	0	0	0	0	-	-	-	-	-	-	-
40	38,816	1	0	7	7	-	0.00257	-	0.01803	0.01803	-	-
42	6,204	5	0	1	1	0	0.08059	-	0.01611	0.01611	-	0
49	12,337	1	0	0	0	-	0.0081	-	-	-	-	-
54	56,321	10	0	6	6	0	0.01775	-	0.01065	0.01065	-	0
66	22,049	0	0	2	2	0	-	-	0.00907	0.00907	-	0
69	13,731	0	1	1	2	0	-	0.00728	0.00728	0.01456	-	0
71	15,754	3	2	1	3	2	0.01904	0.01269	0.00634	0.01904	1:7877	66.67
78	47,033	3	1	10	11	-	0.00637	0.00212	0.02126	0.02338	-	-
82	27,685	1	0	1	1	0	0.00361	-	0.00361	0.00361	-	0
全体	833,389	73	15	61	76	5	0.00875	0.00179	0.00731	0.00911	1:166678	6.58
						max	0.08059	0.01269	0.04215	0.04215		66.67
						min	0.00243	0.00182	0.00182	0.00243		0

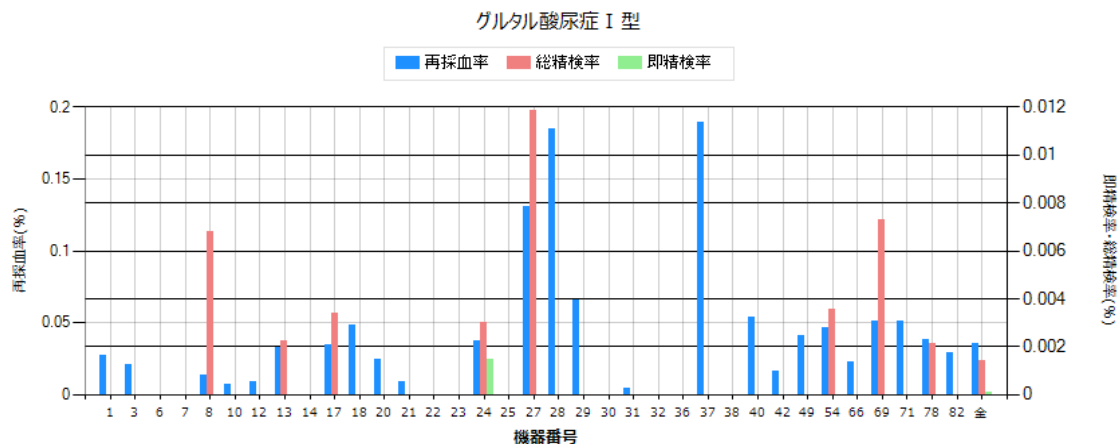


機器No.□	検体数□	再採血数	即精検数	再採血後 精検数	総精検数	発見患者数	再採血率	即精検率	再採血後 精検率	総精検率	発見頻度	陽性適中率 (PPV)
1	54,891	15	0	0	0	0	0.02732	-	-	-	-	-
3	19,159	4	0	0	0	0	0.02087	-	-	-	-	-
6	8,759	0	0	0	0	-	-	-	-	-	-	-
7	11,652	0	0	0	0	0	-	-	-	-	-	-
8	14,660	2	0	1	1	0	0.01364	-	0.00682	0.00682	-	0
10	13,710	1	0	0	0	-	0.00729	-	-	-	-	-
12	11,270	1	0	0	0	0	0.00887	-	-	-	-	-
13	89,550	29	0	2	2	1	0.03238	-	0.00223	0.00223	1:89550	50
14	39,815	0	0	0	0	0	-	-	-	-	-	-
17	58,597	20	0	2	2	-	0.03413	-	0.00341	0.00341	-	-
18	41,136	20	0	0	0	-	0.04861	-	-	-	-	-
20	12,480	3	0	0	0	0	0.02403	-	-	-	-	-
21	10,798	1	0	0	0	-	0.00926	-	-	-	-	-
22	6,680	0	0	0	0	-	-	-	-	-	-	-
23	13,548	0	0	0	0	0	-	-	-	-	-	-
24	66,779	25	1	1	2	-	0.03743	0.00149	0.00149	0.00299	-	-
25	6,683	0	0	0	0	-	-	-	-	-	-	-
27	8,444	11	0	1	1	0	0.13027	-	0.01184	0.01184	-	0
28	17,318	32	0	0	0	0	0.18477	-	-	-	-	-
29	22,886	15	0	0	0	0	0.06554	-	-	-	-	-
30	9,489	0	0	0	0	-	-	-	-	-	-	-
31	24,766	1	0	0	0	0	0.00403	-	-	-	-	-
32	4,702	0	0	0	0	0	-	-	-	-	-	-
36	12,425	0	0	0	0	-	-	-	-	-	-	-
37	7,905	15	0	0	0	-	0.18975	-	-	-	-	-
38	5,357	0	0	0	0	-	-	-	-	-	-	-
40	38,816	21	0	0	0	-	0.0541	-	-	-	-	-
42	6,204	1	0	0	0	0	0.01611	-	-	-	-	-
49	12,337	5	0	0	0	0	0.04052	-	-	-	-	-
54	56,321	26	0	2	2	0	0.04616	-	0.00355	0.00355	-	0
66	22,049	5	0	0	0	0	0.02267	-	-	-	-	-
69	13,731	7	0	1	1	0	0.05097	-	0.00728	0.00728	-	0
71	15,754	8	0	0	0	0	0.05078	-	-	-	-	-
78	47,033	18	0	1	1	-	0.03827	-	0.00212	0.00212	-	-
82	27,685	8	0	0	0	0	0.02889	-	-	-	-	-
全体	833,389	294	1	11	12	1	0.03527	0.00011	0.00131	0.00143	1:833389	8.33
						max	0.18975	0.00149	0.01184	0.01184		50
						min	0.00403	0.00149	0.00149	0.00212		0

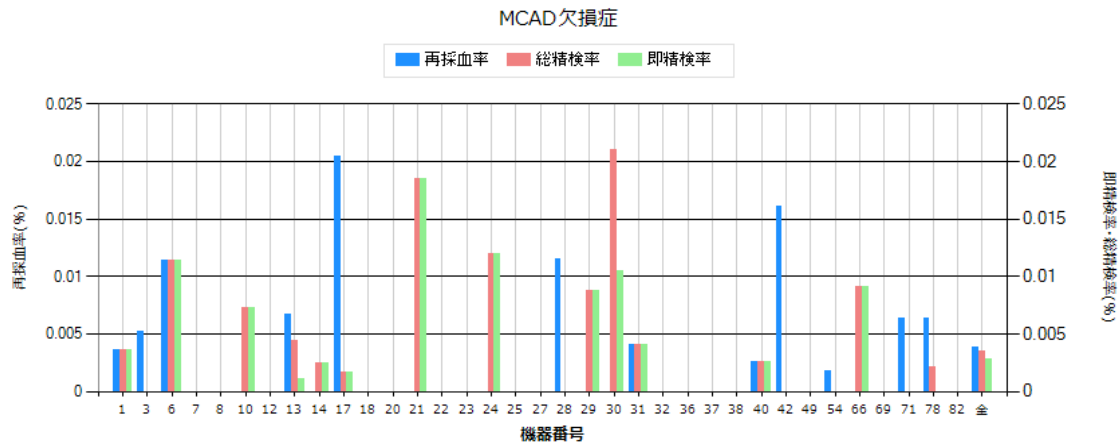


機器No.□	検体数□	再採血数	即精検数	再採血後 精検数	総精検数	発見患者数	再採血率	即精検率	再採血後 精検率	総精検率	発見頻度	陽性適中率 (PPV)
1	54,891	2	2	0	2	0	0.00364	0.00364	-	0.00364	-	0
3	19,159	1	0	0	0	0	0.00521	-	-	-	-	-
6	8,759	1	1	0	1	-	0.01141	0.01141	-	0.01141	-	-
7	11,652	0	0	0	0	0	-	-	-	-	-	-
8	14,660	0	0	0	0	0	-	-	-	-	-	-
10	13,710	0	1	0	1	1	-	0.00729	-	0.00729	1:13710	100
12	11,270	0	0	0	0	0	-	-	-	-	-	-
13	89,550	6	1	3	4	-	0.0067	0.00111	0.00335	0.00446	-	-
14	39,815	0	1	0	1	1	-	0.00251	-	0.00251	1:39815	100
17	58,597	12	1	0	1	-	0.02047	0.0017	-	0.0017	-	-
18	41,136	0	0	0	0	-	-	-	-	-	-	-
20	12,480	0	0	0	0	0	-	-	-	-	-	-
21	10,798	0	2	0	2	-	-	0.01852	-	0.01852	-	-
22	6,680	0	0	0	0	-	-	-	-	-	-	-
23	13,548	0	0	0	0	0	-	-	-	-	-	-
24	66,779	0	8	0	8	-	-	0.01197	-	0.01197	-	-
25	6,683	0	0	0	0	-	-	-	-	-	-	-
27	8,444	0	0	0	0	0	-	-	-	-	-	-
28	17,318	2	0	0	0	0	0.01154	-	-	-	-	-
29	22,886	0	2	0	2	0	-	0.00873	-	0.00873	-	0
30	9,489	0	1	1	2	-	-	0.01053	0.01053	0.02107	-	-
31	24,766	1	1	0	1	0	0.00403	0.00403	-	0.00403	-	0
32	4,702	0	0	0	0	0	-	-	-	-	-	-
36	12,425	0	0	0	0	-	-	-	-	-	-	-
37	7,905	0	0	0	0	-	-	-	-	-	-	-
38	5,357	0	0	0	0	-	-	-	-	-	-	-
40	38,816	1	1	0	1	1	0.00257	0.00257	-	0.00257	1:38816	100
42	6,204	1	0	0	0	0	0.01611	-	-	-	-	-
49	12,337	0	0	0	0	-	-	-	-	-	-	-
54	56,321	1	0	0	0	0	0.00177	-	-	-	-	-
66	22,049	0	2	0	2	2	-	0.00907	-	0.00907	1:11025	100
69	13,731	0	0	0	0	0	-	-	-	-	-	-
71	15,754	1	0	0	0	0	0.00634	-	-	-	-	-
78	47,033	3	0	1	1	1	0.00637	-	0.00212	0.00212	1:47033	100
82	27,685	0	0	0	0	0	-	-	-	-	-	-
全体	833,389	32	24	5	29	6	0.00383	0.00287	0.00059	0.00347	1:138898	20.69
						max	0.02047	0.01852	0.01053	0.02107		100
						min	0.00177	0.00111	0.00212	0.0017		0

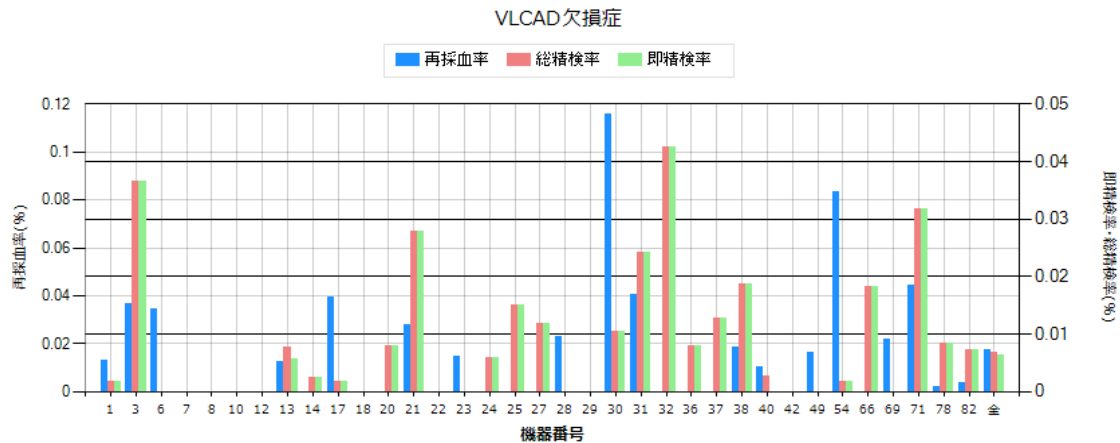


機器No.□	検体数□	再採血数	即精検数	再採血後 精検数	総精検数	発見患者数	再採血率	即精検率	再採血後 精検率	総精検率	発見頻度	陽性適中率 (PPV)
1	54,891	7	1	0	1	0	0.01275	0.00182	-	0.00182	-	0
3	19,159	7	7	0	7	0	0.03653	0.03653	-	0.03653	-	0
6	8,759	3	0	0	0	-	0.03425	-	-	-	-	-
7	11,652	0	0	0	0	0	-	-	-	-	-	-
8	14,660	0	0	0	0	0	-	-	-	-	-	-
10	13,710	0	0	0	0	-	-	-	-	-	-	-
12	11,270	0	0	0	0	0	-	-	-	-	-	-
13	89,550	11	5	2	7	6	0.01228	0.00558	0.00223	0.00781	1:14925	85.71
14	39,815	0	1	0	1	0	-	0.00251	-	0.00251	-	0
17	58,597	23	1	0	1	-	0.03925	0.0017	-	0.0017	-	-
18	41,136	0	0	0	0	-	-	-	-	-	-	-
20	12,480	0	1	0	1	0	-	0.00801	-	0.00801	-	0
21	10,798	3	3	0	3	-	0.02778	0.02778	-	0.02778	-	-
22	6,680	0	0	0	0	-	-	-	-	-	-	-
23	13,548	2	0	0	0	0	0.01476	-	-	-	-	-
24	66,779	0	4	0	4	-	-	0.00598	-	0.00598	-	-
25	6,683	0	1	0	1	-	-	0.01496	-	0.01496	-	-
27	8,444	0	1	0	1	1	-	0.01184	-	0.01184	1:8444	100
28	17,318	4	0	0	0	0	0.02309	-	-	-	-	-
29	22,886	0	0	0	0	0	-	-	-	-	-	-
30	9,489	11	1	0	1	-	0.11592	0.01053	-	0.01053	-	-
31	24,766	10	6	0	6	0	0.04037	0.02422	-	0.02422	-	0
32	4,702	0	2	0	2	0	-	0.04253	-	0.04253	-	0
36	12,425	0	1	0	1	-	-	0.00804	-	0.00804	-	-
37	7,905	0	1	0	1	0	-	0.01265	-	0.01265	-	0
38	5,357	1	1	0	1	1	0.01866	0.01866	-	0.01866	1:5357	100
40	38,816	4	0	1	1	1	0.0103	-	0.00257	0.00257	1:38816	100
42	6,204	0	0	0	0	0	-	-	-	-	-	-
49	12,337	2	0	0	0	0	0.01621	-	-	-	-	-
54	56,321	47	1	0	1	0	0.08345	0.00177	-	0.00177	-	0
66	22,049	0	4	0	4	1	-	0.01814	-	0.01814	1:22049	25
69	13,731	3	0	0	0	0	0.02184	-	-	-	-	-
71	15,754	7	5	0	5	-	0.04443	0.03173	-	0.03173	-	-
78	47,033	1	4	0	4	-	0.00212	0.0085	-	0.0085	-	-
82	27,685	1	2	0	2	0	0.00361	0.00722	-	0.00722	-	0
全体	833,389	147	53	3	56	10	0.01763	0.00635	0.00035	0.00671	1:83339	17.86
						max	0.11592	0.04253	0.00257	0.04253		100
						min	0.00212	0.0017	0.00223	0.0017		0

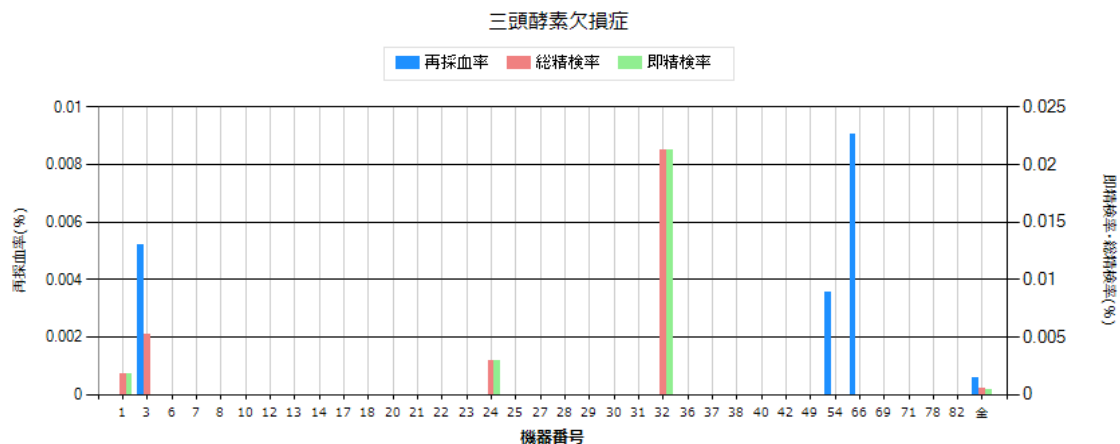

機器No.□	検体数□	再採血数	即精検数	再採血後 精検数	総精検数	発見患者数	再採血率	即精検率	再採血後 精検率	総精検率	発見頻度	陽性適中率 (PPV)
1	54,891	0	1	0	1	0	-	0.00182	-	0.00182	-	0
3	19,159	1	0	1	1	0	0.00521	-	0.00521	0.00521	-	0
6	8,759	0	0	0	0	-	-	-	-	-	-	-
7	11,652	0	0	0	0	0	-	-	-	-	-	-
8	14,660	0	0	0	0	0	-	-	-	-	-	-
10	13,710	0	0	0	0	-	-	-	-	-	-	-
12	11,270	0	0	0	0	0	-	-	-	-	-	-
13	89,550	0	0	0	0	-	-	-	-	-	-	-
14	39,815	0	0	0	0	0	-	-	-	-	-	-
17	58,597	0	0	0	0	-	-	-	-	-	-	-
18	41,136	0	0	0	0	-	-	-	-	-	-	-
20	12,480	0	0	0	0	0	-	-	-	-	-	-
21	10,798	0	0	0	0	-	-	-	-	-	-	-
22	6,680	0	0	0	0	-	-	-	-	-	-	-
23	13,548	0	0	0	0	0	-	-	-	-	-	-
24	66,779	-	2	0	2	-	-	0.00299	-	0.00299	-	-
25	6,683	0	0	0	0	-	-	-	-	-	-	-
27	8,444	0	0	0	0	0	-	-	-	-	-	-
28	17,318	0	0	0	0	0	-	-	-	-	-	-
29	22,886	0	0	0	0	0	-	-	-	-	-	-
30	9,489	0	0	0	0	-	-	-	-	-	-	-
31	24,766	0	0	0	0	0	-	-	-	-	-	-
32	4,702	0	1	0	1	0	-	0.02126	-	0.02126	-	0
36	12,425	0	0	0	0	-	-	-	-	-	-	-
37	7,905	0	0	0	0	-	-	-	-	-	-	-
38	5,357	0	0	0	0	-	-	-	-	-	-	-
40	38,816	0	0	0	0	-	-	-	-	-	-	-
42	6,204	0	0	0	0	0	-	-	-	-	-	-
49	12,337	0	0	0	0	-	-	-	-	-	-	-
54	56,321	2	0	0	0	0	0.00355	-	-	-	-	-
66	22,049	2	0	0	0	0	0.00907	-	-	-	-	-
69	13,731	0	0	0	0	0	-	-	-	-	-	-
71	15,754	0	0	0	0	0	-	-	-	-	-	-
78	47,033	0	0	0	0	-	-	-	-	-	-	-
82	27,685	0	0	0	0	0	-	-	-	-	-	-
全体	833,389	5	4	1	5	0	0.00059	0.00047	0.00011	0.00059	-	0
						max	0.00907	0.02126	0.00521	0.02126		0
						min	0.00355	0.00182	0.00521	0.00182		0

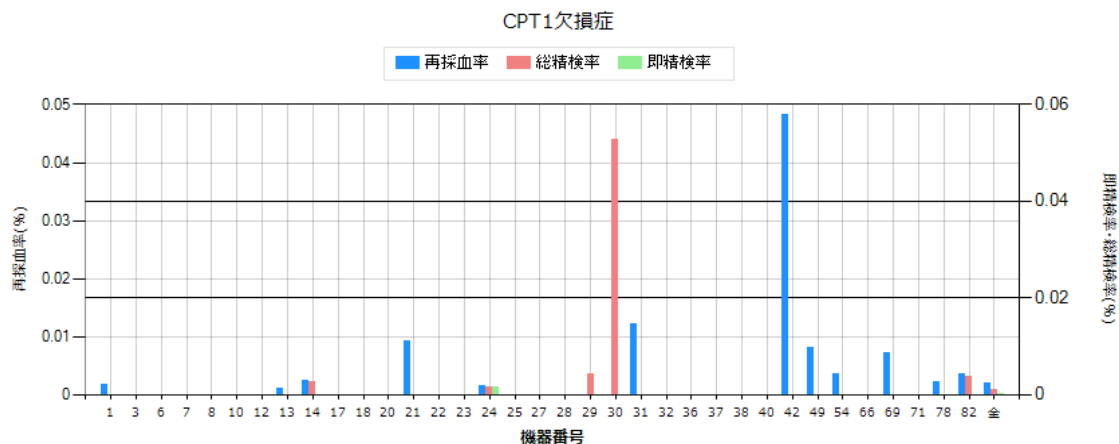

機器No.□	検体数□	再採血数	即精検数	再採血後 精検数	総精検数	発見患者数	再採血率	即精検率	再採血後 精検率	総精検率	発見頻度	陽性適中率 (PPV)
1	54,891	1	0	0	0	0	0.00182	-	-	-	-	-
3	19,159	0	0	0	0	0	-	-	-	-	-	-
6	8,759	0	0	0	0	-	-	-	-	-	-	-
7	11,652	0	0	0	0	0	-	-	-	-	-	-
8	14,660	0	0	0	0	0	-	-	-	-	-	-
10	13,710	0	0	0	0	-	-	-	-	-	-	-
12	11,270	0	0	0	0	0	-	-	-	-	-	-
13	89,550	1	0	0	0	-	0.00111	-	-	-	-	-
14	39,815	1	0	1	1	0	0.00251	-	0.00251	0.00251	-	0
17	58,597	0	0	0	0	-	-	-	-	-	-	-
18	41,136	0	0	0	0	-	-	-	-	-	-	-
20	12,480	0	0	0	0	0	-	-	-	-	-	-
21	10,798	1	0	0	0	-	0.00926	-	-	-	-	-
22	6,680	0	0	0	0	-	-	-	-	-	-	-
23	13,548	0	0	0	0	0	-	-	-	-	-	-
24	66,779	1	1	0	1	-	0.00149	0.00149	-	0.00149	-	-
25	6,683	0	0	0	0	-	-	-	-	-	-	-
27	8,444	0	0	0	0	0	-	-	-	-	-	-
28	17,318	0	0	0	0	0	-	-	-	-	-	-
29	22,886	0	0	1	1	0	-	-	0.00436	0.00436	-	0
30	9,489	0	0	5	5	-	-	-	0.05269	0.05269	-	-
31	24,766	3	0	0	0	0	0.01211	-	-	-	-	-
32	4,702	0	0	0	0	0	-	-	-	-	-	-
36	12,425	0	0	0	0	-	-	-	-	-	-	-
37	7,905	0	0	0	0	-	-	-	-	-	-	-
38	5,357	0	0	0	0	-	-	-	-	-	-	-
40	38,816	0	0	0	0	-	-	-	-	-	-	-
42	6,204	3	0	0	0	0	0.04835	-	-	-	-	-
49	12,337	1	0	0	0	0	0.0081	-	-	-	-	-
54	56,321	2	0	0	0	0	0.00355	-	-	-	-	-
66	22,049	0	0	0	0	0	-	-	-	-	-	-
69	13,731	1	0	0	0	0	0.00728	-	-	-	-	-
71	15,754	0	0	0	0	0	-	-	-	-	-	-
78	47,033	1	0	0	0	-	0.00212	-	-	-	-	-
82	27,685	1	0	1	1	0	0.00361	-	0.00361	0.00361	-	0
全体	833,389	17	1	8	9	0	0.00203	0.00011	0.00095	0.00107	-	0
						max	0.04835	0.00149	0.05269	0.05269		0
						min	0.00111	0.00149	0.00251	0.00149		0

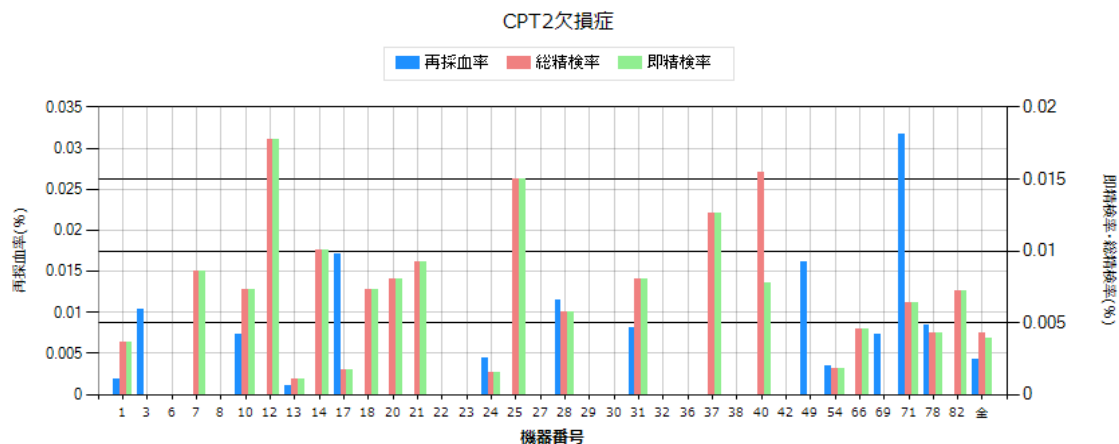

機器No.□	検体数□	再採血数	即精検数	再採血後 精検数	総精検数	発見患者数	再採血率	即精検率	再採血後 精検率	総精検率	発見頻度	陽性適中率 (PPV)
1	54,891	1	2	0	2	0	0.00182	0.00364	-	0.00364	-	0
3	19,159	2	0	0	0	0	0.01043	-	-	-	-	-
6	8,759	0	0	0	0	-	-	-	-	-	-	-
7	11,652	0	1	0	1	0	-	0.00858	-	0.00858	-	0
8	14,660	0	0	0	0	0	-	-	-	-	-	-
10	13,710	1	1	0	1	0	0.00729	0.00729	-	0.00729	-	0
12	11,270	0	2	0	2	0	-	0.01774	-	0.01774	-	0
13	89,550	1	1	0	1	-	0.00111	0.00111	-	0.00111	-	-
14	39,815	0	4	0	4	1	-	0.01004	-	0.01004	1:39815	25
17	58,597	10	1	0	1	-	0.01706	0.0017	-	0.0017	-	-
18	41,136	0	3	0	3	-	-	0.00729	-	0.00729	-	-
20	12,480	0	1	0	1	0	-	0.00801	-	0.00801	-	0
21	10,798	0	1	0	1	-	-	0.00926	-	0.00926	-	-
22	6,680	0	0	0	0	-	-	-	-	-	-	-
23	13,548	0	0	0	0	0	-	-	-	-	-	-
24	66,779	3	1	0	1	-	0.00449	0.00149	-	0.00149	-	-
25	6,683	0	1	0	1	-	-	0.01496	-	0.01496	-	-
27	8,444	0	0	0	0	0	-	-	-	-	-	-
28	17,318	2	1	0	1	0	0.01154	0.00577	-	0.00577	-	0
29	22,886	0	0	0	0	0	-	-	-	-	-	-
30	9,489	0	0	0	0	-	-	-	-	-	-	-
31	24,766	2	2	0	2	0	0.00807	0.00807	-	0.00807	-	0
32	4,702	0	0	0	0	0	-	-	-	-	-	-
36	12,425	0	0	0	0	-	-	-	-	-	-	-
37	7,905	0	1	0	1	0	-	0.01265	-	0.01265	-	0
38	5,357	0	0	0	0	-	-	-	-	-	-	-
40	38,816	0	3	3	6	-	-	0.00772	0.00772	0.01545	-	-
42	6,204	0	0	0	0	0	-	-	-	-	-	-
49	12,337	2	0	0	0	0	0.01621	-	-	-	-	-
54	56,321	2	1	0	1	0	0.00355	0.00177	-	0.00177	-	0
66	22,049	0	1	0	1	0	-	0.00453	-	0.00453	-	0
69	13,731	1	0	0	0	0	0.00728	-	-	-	-	-
71	15,754	5	1	0	1	0	0.03173	0.00634	-	0.00634	-	0
78	47,033	4	2	0	2	-	0.0085	0.00425	-	0.00425	-	-
82	27,685	0	2	0	2	1	-	0.00722	-	0.00722	1:27685	50
全体	833,389	36	33	3	36	2	0.00431	0.00395	0.00035	0.00431	1:416694	5.56
						max	0.03173	0.01774	0.00772	0.01774		50
						min	0.00111	0.00111	0.00772	0.00111		0