




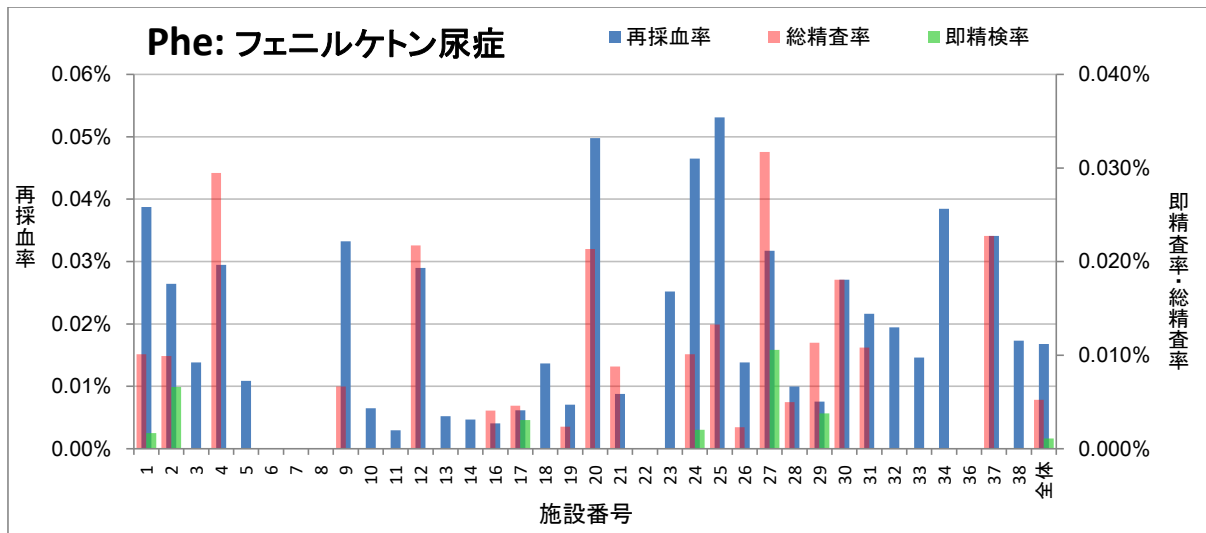


施設 No	検体数	項目	カットオフ値		再採 血数	即精 検数	再採血後 精検数	総精 検数	発見 患者数	再採血率	即精検率	再採血後 精検率	総精査率	発見頻度	陽性適中率 (PPV)
			初回 検査	即精査											
1	59,384	Phe	120.00	600.00	23	1	5	6	4	0.039%	0.002%	0.008%	0.010%	1:14,846	66.67%
2	60,537	Phe	120.00	300.00	16	4	2	6	2	0.026%	0.007%	0.003%	0.010%	1:30,269	33.33%
3	21,662	Phe	120.00	600.00	3	0	0	0	0	0.014%	-	-	-	-	-
4	6,785	Phe	180.00	600.00	2	0	2	2	0	0.029%	-	0.029%	0.029%	-	0.00%
5	18,393	Phe	180.00	600.00	2	0	0	0	0	0.011%	-	-	-	-	-
6	9,988	Phe	110.00	-	0	0	0	0	0	-	-	-	-	-	-
7	14,110	Phe	180.00	600.00	-	-	-	0	-	-	-	-	-	-	-
8	15,661	Phe	181.00	600.00	0	0	0	0	0	-	-	-	-	-	-
9	15,038	Phe	120.00	300.00	5	0	1	1	1	0.033%	-	0.007%	0.007%	1:15,038	100.00%
10	15,369	Phe	150.00	600.00	1	0	0	0	0	0.007%	-	-	-	-	-
11	33,562	Phe	180.00	600.00	1	0	0	0	0	0.003%	-	-	-	-	-
12	13,801	Phe	120.00	480.00	4	0	3	3	0	0.029%	-	0.022%	0.022%	-	0.00%
13	95,832	Phe	180.00	360.00	5	0	0	0	0	0.005%	-	-	-	-	-
14	42,573	Phe	130.00	600.00	2	-	-	0	0	0.005%	-	-	-	-	-
16	24,488	Phe	120.00	500.00	1	0	1	1	1	0.004%	-	0.004%	0.004%	-	0.00%
17	65,106	Phe	180.00	600.00	4	2	1	3	3	0.006%	0.003%	0.002%	0.005%	-	0.00%
18	43,919	Phe	150.00	600.00	6	0	0	0	0	0.014%	-	-	-	-	-
19	42,358	Phe	150.00	600.00	3	-	1	1	1	0.007%	-	0.002%	0.002%	-	0.00%
20	14,058	Phe	120.00	-	7	0	3	3	3	0.050%	-	0.021%	0.021%	1:4,686	100.00%
21	11,372	Phe	120.00	600.00	1	0	1	1	0	0.009%	-	0.009%	0.009%	-	0.00%
22	7,270	Phe	120.00	600.00	-	-	-	0	-	-	-	-	-	-	-
23	15,864	Phe	150.00	600.00	4	0	0	0	0	0.025%	-	-	-	-	-
24	49,476	Phe	100.00	600.00	23	1	4	5	5	0.046%	0.002%	0.008%	0.010%	-	0.00%
25	7,533	Phe	120.00	500.00	4	0	1	1	0	0.053%	-	0.013%	0.013%	-	0.00%
26	43,346	Phe	120.00	-	6	-	1	1	1	0.014%	-	0.002%	0.002%	-	0.00%
27	9,457	Phe	120.00	600.00	3	1	2	3	1	0.032%	0.011%	0.021%	0.032%	1:9,457	33.33%
28	20,041	Phe	140.00	242.00	2	0	1	1	0	0.010%	-	0.005%	0.005%	-	0.00%
29	26,450	Phe	180.00	600.00	2	1	2	3	2	0.008%	0.004%	0.008%	0.011%	1:13,225	66.67%
30	11,072	Phe	120.00	500.00	3	0	2	2	0	0.027%	-	0.018%	0.018%	-	0.00%
31	27,752	Phe	120.00	-	6	0	3	3	1	0.022%	-	0.011%	0.011%	1:27,752	33.33%
32	5,134	Phe	150.00	600.00	1	0	0	0	0	0.019%	-	-	-	-	-
33	13,684	Phe	120.00	400.00	2	0	0	0	0	0.015%	-	-	-	-	-
34	20,794	Phe	120.00	600.00	8	0	0	0	0	0.038%	-	-	-	-	-
36	14,517	Phe	180.00	-	0	0	0	0	0	-	-	-	-	-	-
37	8,794	Phe	120.00	-	3	0	2	2	0	0.034%	-	0.023%	0.023%	-	0.00%
38	5,772	Phe	130.00	-	1	-	-	0	0	0.017%	-	-	-	-	-
全体	916,724	Phe	139.47	537.31	154	10	38	48	14	0.02%	0.001%	0.004%	0.005%	1:65,480	29.17%
										max	0.053%	0.011%	0.029%	0.032%	100.00%
										min	0.003%	0.002%	0.002%	0.002%	0.00%

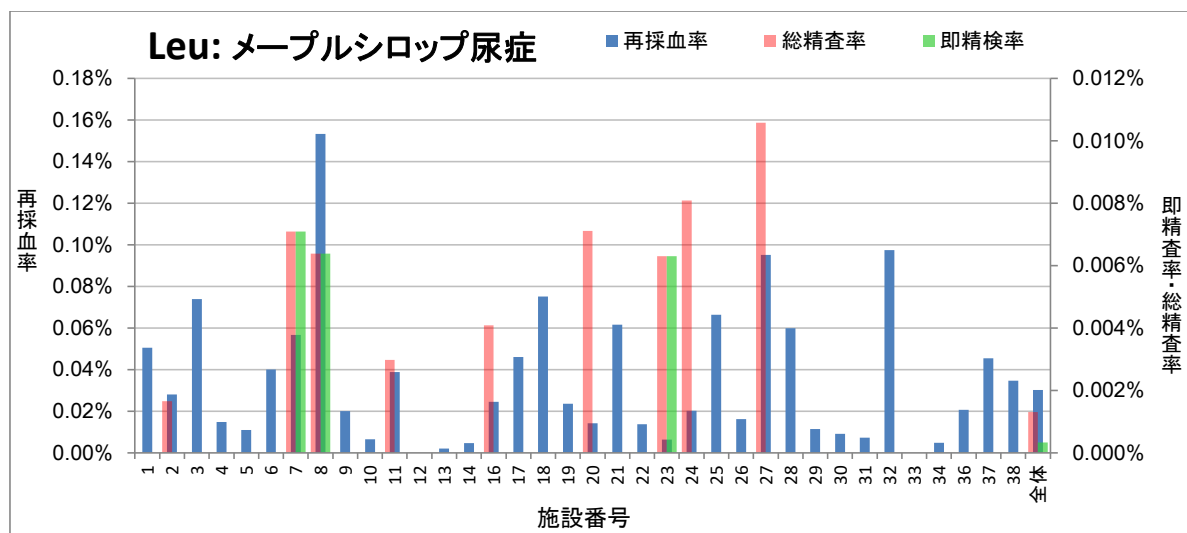


施設 No	検体数	項目	カットオフ値		再採 血数	即精 検数	再採血後 精検数	総精 検数	死 患者 数	再採血率	即精検率	再採血後 精検率	総精査率	発見頻度	陽性適中率 (PPV)
			初回 検査	即精査											
1	59,384	Leu+Ile	350.00	600.00	30	0	0	0	0	0.051%	—	—	—	—	—
2	60,537	Leu+Ile	350.00	600.00	17	0	1	1	0	0.028%	—	0.002%	0.002%	—	0.00%
3	21,662	Leu+Ile	350.00	600.00	16	0	0	0	0	0.074%	—	—	—	—	—
4	6,785	Leu+Ile	350.00	600.00	1	0	0	0	0	0.015%	—	—	—	—	—
5	18,393	Leu+Ile	350.00	600.00	2	0	0	0	0	0.011%	—	—	—	—	—
6	9,988	Leu+Ile	310.00	—	4	0	0	0	0	0.040%	—	—	—	—	—
7	14,110	Leu+Ile	350.00	600.00	8	1	—	1	0	0.057%	0.007%	—	0.007%	—	0.00%
8	15,661	Leu+Ile	256.00	600.00	24	1	0	1	0	0.153%	0.006%	—	0.006%	—	0.00%
9	15,038	Leu+Ile	350.00	700.00	3	0	0	0	0	0.020%	—	—	—	—	—
10	15,369	Leu+Ile	360.00	600.00	1	0	0	0	0	0.007%	—	—	—	—	—
11	33,562	Leu+Ile	350.00	600.00	13	0	1	1	0	0.039%	—	0.003%	0.003%	—	0.00%
12	13,801	Leu+Ile	350.00	600.00	0	0	0	0	0	—	—	—	—	—	—
13	95,832	Leu+Ile	350.00	458.00	2	0	0	0	0	0.002%	—	—	—	—	—
14	42,573	Leu+Ile	350.00	600.00	2	—	—	0	0	0.005%	—	—	—	—	—
16	24,488	Leu+Ile	350.00	600.00	6	—	1	1	0	0.025%	—	0.004%	0.004%	—	0.00%
17	65,106	Leu+Ile	350.00	—	30	0	0	0	0	0.046%	—	—	—	—	—
18	43,919	Leu+Ile	350.00	—	33	0	0	0	0	0.075%	—	—	—	—	—
19	42,358	Leu+Ile	350.00	600.00	10	—	—	0	0	0.024%	—	—	—	—	—
20	14,058	Leu+Ile	350.00	—	2	0	1	1	0	0.014%	—	0.007%	0.007%	—	0.00%
21	11,372	Leu+Ile	280.00	600.00	7	0	0	0	0	0.062%	—	—	—	—	—
22	7,270	Leu+Ile	350.00	600.00	1	—	—	0	0	0.014%	—	—	—	—	—
23	15,864	Leu+Ile	360.00	478.00	1	1	0	1	0	0.006%	0.006%	—	0.006%	—	0.00%
24	49,476	Leu+Ile	350.00	600.00	10	0	4	4	0	0.020%	—	0.008%	0.008%	—	0.00%
25	7,533	Leu+Ile	315.00	600.00	5	0	0	0	0	0.066%	—	—	—	—	—
26	43,346	Leu+Ile	350.00	—	7	—	—	0	0	0.016%	—	—	—	—	—
27	9,457	Leu+Ile	360.00	600.00	9	0	1	1	0	0.095%	—	0.011%	0.011%	—	0.00%
28	20,041	Leu+Ile	360.00	600.00	12	0	0	0	0	0.060%	—	—	—	—	—
29	26,450	Leu+Ile	380.00	600.00	3	0	0	0	0	0.011%	—	—	—	—	—
30	11,072	Leu+Ile	350.00	600.00	1	0	0	0	0	0.009%	—	—	—	—	—
31	27,752	Leu+Ile	350.00	—	2	0	0	0	0	0.007%	—	—	—	—	—
32	5,134	Leu+Ile	360.00	600.00	5	0	0	0	0	0.097%	—	—	—	—	—
33	13,684	Leu+Ile	350.00	600.00	0	0	0	0	0	—	—	—	—	—	—
34	20,794	Leu+Ile	320.00	600.00	1	0	0	0	0	0.005%	—	—	—	—	—
36	14,517	Leu+Ile	350.00	—	3	0	0	0	0	0.021%	—	—	—	—	—
37	8,794	Leu+Ile	350.00	—	4	0	0	0	0	0.045%	—	—	—	—	—
38	5,772	Leu+Ile	350.00	—	2	—	—	0	0	0.035%	—	—	—	—	—
全体	916,724	Leu+Ile	344.75	593.93	277	3	9	12	0	0.03%	0.000%	0.001%	0.001%	—	0.00%
										max	0.153%	0.007%	0.011%	0.011%	0.00%
										min	0.002%	0.006%	0.002%	0.002%	0.00%

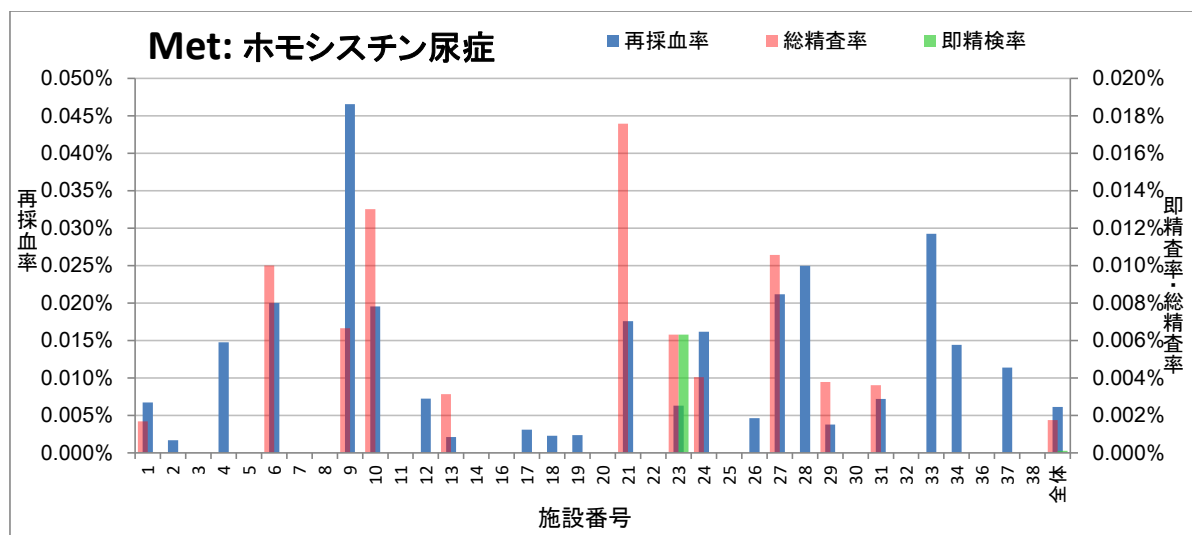


施設 No	検体数	項目	カットオフ値		再採 血数	即精 査数	再採血後 精査数	総精 査数	元元 患者 数	再採血率	即精査率	再採血後 精査率	総精査率	発見頻度	陽性適中率 (PPV)
			初回 検査	即精査											
1	59,384	Met	70.00	100.00	4	0	1	1	0	0.007%	—	0.002%	0.002%	—	0.00%
2	60,537	Met	70.00	240.00	1	0	0	0	0	0.002%	—	—	—	—	—
3	21,662	Met	70.00	100.00	0	0	0	0	0	—	—	—	—	—	—
4	6,785	Met	80.00	—	1	0	0	0	0	0.015%	—	—	—	—	—
5	18,393	Met	80.00	100.00	0	0	0	0	—	—	—	—	—	—	—
6	9,988	Met	50.00	—	2	0	1	1	0	0.020%	—	0.010%	0.010%	—	0.00%
7	14,110	Met	80.00	—	—	—	—	0	—	—	—	—	—	—	—
8	15,661	Met	67.00	—	0	0	0	0	0	—	—	—	—	—	—
9	15,038	Met	50.00	100.00	7	0	1	1	0	0.047%	—	0.007%	0.007%	—	0.00%
10	15,369	Met	60.00	—	3	0	2	2	0	0.020%	—	0.013%	0.013%	—	0.00%
11	33,562	Met	80.00	—	0	0	0	0	0	—	—	—	—	—	—
12	13,801	Met	67.00	—	1	0	0	0	0	0.007%	—	—	—	—	—
13	95,832	Met	100.00	268.00	2	0	3	3	0	0.002%	—	0.003%	0.003%	—	0.00%
14	42,573	Met	80.00	—	—	—	—	0	—	—	—	—	—	—	—
16	24,488	Met	70.00	340.00	—	—	—	0	—	—	—	—	—	—	—
17	65,106	Met	70.00	—	2	0	0	0	0	0.003%	—	—	—	—	—
18	43,919	Met	80.00	—	1	0	0	0	0	0.002%	—	—	—	—	—
19	42,358	Met	70.00	—	1	—	—	0	0	0.002%	—	—	—	—	—
20	14,058	Met	80.00	—	0	0	0	0	0	—	—	—	—	—	—
21	11,372	Met	50.00	100.00	2	0	2	2	0	0.018%	—	0.018%	0.018%	—	0.00%
22	7,270	Met	67.00	100.00	—	—	—	0	—	—	—	—	—	—	—
23	15,864	Met	60.00	—	1	1	0	1	0	0.006%	0.006%	—	0.006%	—	0.00%
24	49,476	Met	50.00	—	8	0	2	2	0	0.016%	—	0.004%	0.004%	—	0.00%
25	7,533	Met	67.00	340.00	0	0	0	0	0	—	—	—	—	—	—
26	43,346	Met	70.00	—	2	—	—	0	0	0.005%	—	—	—	—	—
27	9,457	Met	60.00	—	2	0	1	1	0	0.021%	—	0.011%	0.011%	—	0.00%
28	20,041	Met	60.00	134.00	5	0	0	0	0	0.025%	—	—	—	—	—
29	26,450	Met	80.00	—	1	0	1	1	0	0.004%	—	0.004%	0.004%	—	0.00%
30	11,072	Met	70.00	100.00	0	0	0	0	0	—	—	—	—	—	—
31	27,752	Met	70.00	—	2	0	1	1	0	0.007%	—	0.004%	0.004%	—	0.00%
32	5,134	Met	60.00	—	0	0	0	0	0	—	—	—	—	—	—
33	13,684	Met	50.00	—	4	0	0	0	0	0.029%	—	—	—	—	—
34	20,794	Met	80.00	—	3	0	0	0	0	0.014%	—	—	—	—	—
36	14,517	Met	80.00	—	0	0	0	0	0	—	—	—	—	—	—
37	8,794	Met	60.00	—	1	0	0	0	0	0.011%	—	—	—	—	—
38	5,772	Met	80.00	—	—	—	—	0	—	—	—	—	—	—	—
全体	916,724	Met	69.11	168.50	56	1	15	16	0	0.01%	0.000%	0.002%	0.002%	—	0.00%
										max	0.047%	0.006%	0.018%	0.018%	0.00%
										min	0.002%	0.006%	0.002%	0.002%	0.00%

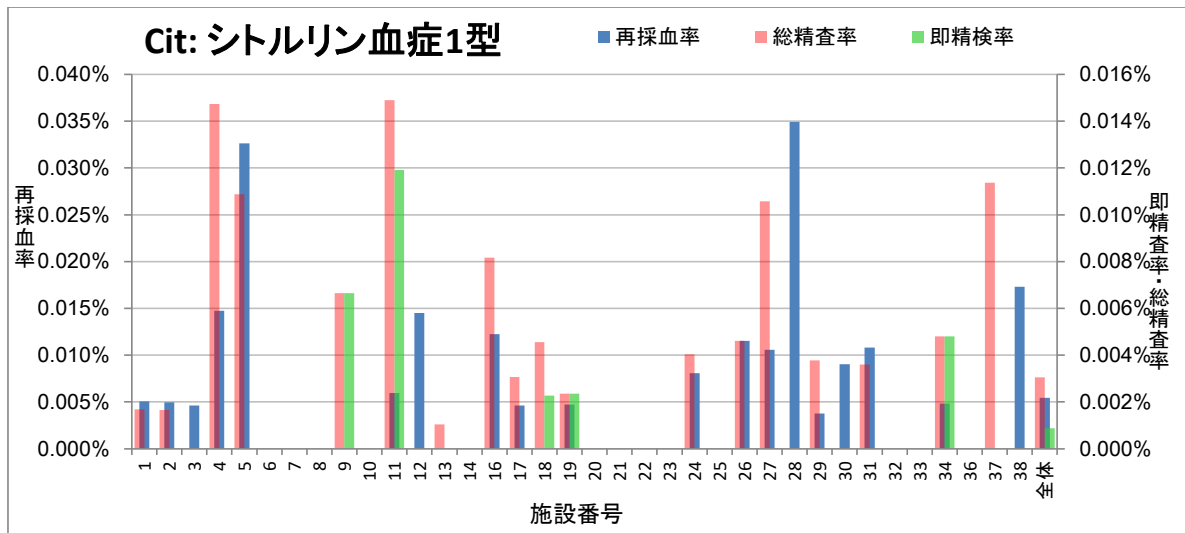


施設 No	検体数	項目	カットオフ値		再採 血数	即精 検数	再採血後 精検数	総精 検数	発 見 患 者 数	再採血率	即精検率	再採血後 精検率	総精査率	発見頻度	陽性適中率 (PPV)
			初回 検査	即精査											
1	59,384	Cit	70.00	300.00	3	0	1	1	0	0.005%	—	0.002%	0.002%	—	0.00%
2	60,537	Cit	80.00	300.00	3	0	1	1	0	0.005%	—	0.002%	0.002%	—	0.00%
3	21,662	Cit	80.00	200.00	1	0	0	0	0	0.005%	—	—	—	—	—
4	6,785	Cit	90.00	270.00	1	0	1	1	0	0.015%	—	0.015%	0.015%	—	0.00%
5	18,393	Cit	100.00	300.00	6	0	2	2	—	0.033%	—	0.011%	0.011%	—	0.00%
6	9,988	Cit	50.00	250.00	0	0	0	0	0	—	—	—	—	—	—
7	14,110	Cit	100.00	300.00	—	—	—	0	—	—	—	—	—	—	—
8	15,661	Cit	68.00	300.00	0	0	0	0	0	—	—	—	—	—	—
9	15,038	Cit/AA	0.03	※2	0	1	0	1	1	—	0.007%	—	0.007%	1: 15,038	100.00%
10	15,369	Cit	85.00	300.00	0	0	0	0	0	—	—	—	—	—	—
11	33,562	Cit	—	80.00	2	4	1	5	1	0.006%	0.012%	0.003%	0.015%	1: 33,562	20.00%
12	13,801	Cit	55.00	80.00	2	0	0	0	0	0.014%	—	—	—	—	—
13	95,832	Cit	100.00	200.00	0	0	1	1	0	—	—	0.001%	0.001%	—	0.00%
14	42,573	Cit	80.00	300.00	—	—	—	0	—	—	—	—	—	—	—
16	24,488	Cit	80.00	300.00	3	—	2	2	—	0.012%	—	0.008%	0.008%	—	0.00%
17	65,106	Cit	50.00	300.00	3	0	2	2	—	0.005%	—	0.003%	0.003%	—	0.00%
18	43,919	Cit	100.00	—	—	1	1	2	1	—	0.002%	0.002%	0.005%	1: 43,919	50.00%
19	42,358	Cit	80.00	140.00	2	1	—	1	—	0.005%	0.002%	—	0.002%	—	0.00%
20	14,058	Cit	100.00	—	0	0	0	0	0	—	—	—	—	—	—
21	11,372	Cit	40.00	300.00	0	0	0	0	0	—	—	—	—	—	—
22	7,270	Cit	65.00	300.00	—	—	—	0	—	—	—	—	—	—	—
23	15,864	Cit	85.00	300.00	0	0	0	0	0	—	—	—	—	—	—
24	49,476	Cit	100.00	300.00	4	0	2	2	—	0.008%	—	0.004%	0.004%	—	0.00%
25	7,533	Cit	100.00	250.00	0	0	0	0	0	—	—	—	—	—	—
26	43,346	Cit	60.00	300.00	5	—	2	2	—	0.012%	—	0.005%	0.005%	—	0.00%
27	9,457	Cit	85.00	300.00	1	0	1	1	0	0.011%	—	0.011%	0.011%	—	0.00%
28	20,041	Cit	65.00	300.00	7	0	0	0	0	0.035%	—	—	—	—	—
29	26,450	Cit	100.00	300.00	1	0	1	1	0	0.004%	—	0.004%	0.004%	—	0.00%
30	11,072	Cit	100.00	300.00	1	0	0	0	0	0.009%	—	—	—	—	—
31	27,752	Cit	60.00	300.00	3	0	1	1	—	0.011%	—	0.004%	0.004%	—	0.00%
32	5,134	Cit	85.00	300.00	0	0	0	0	0	—	—	—	—	—	—
33	13,684	Cit	60.00	180.00	0	0	0	0	0	—	—	—	—	—	—
34	20,794	Cit	85.00	300.00	1	1	0	1	—	0.005%	0.005%	—	0.005%	—	0.00%
36	14,517	Cit	100.00	—	0	0	0	0	0	—	—	—	—	—	—
37	8,794	Cit	85.00	—	0	0	1	1	1	—	—	0.011%	0.011%	1: 8,794	100.00%
38	5,772	Cit	100.00	250.00	1	—	—	0	—	0.017%	—	—	—	—	—
全体	916,724	Cit	78.37	264.52	50	8	20	28	4	0.01%	0.001%	0.002%	0.003%	1: 229,181	14.286%
※2 Cit>100										max	0.035%	0.012%	0.015%	—	100.00%
										min	0.004%	0.002%	0.001%	—	0.00%

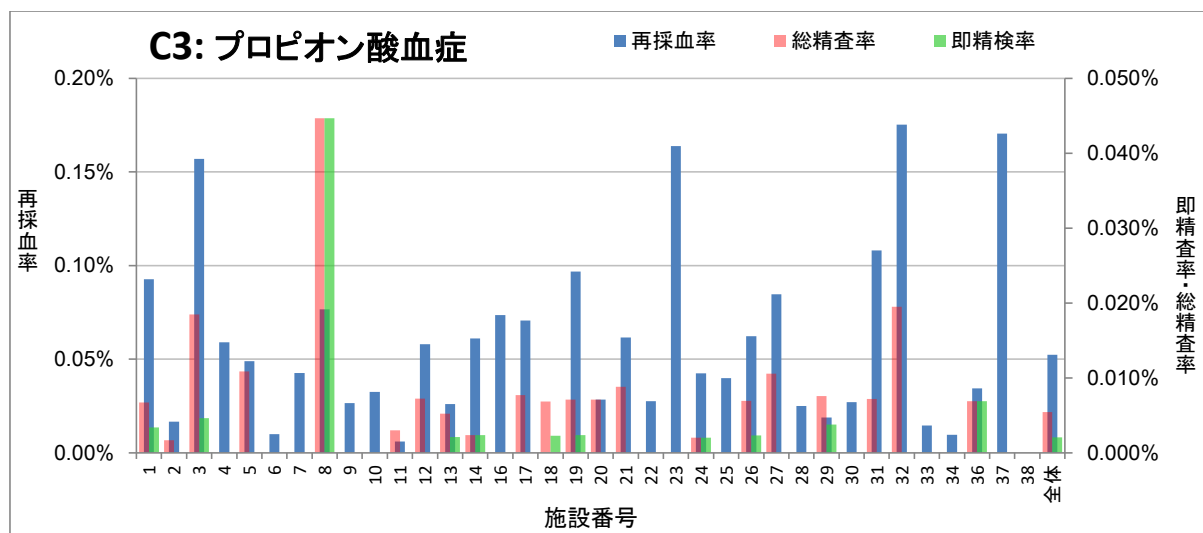


施設 No	検体数	項目	カットオフ値		再採 血数	即精 検数	再採血後 精検数	総精 検数	発見 患者 数	再採血率	即精検率	再採血後 精検率	総精査率	発見頻度	陽性適中率 (PPV)
			初回 検査	即精査											
1	59,384	C3	4.00	8.00	55	2	2	4	0	0.093%	0.003%	0.003%	0.007%	—	0.00%
2	60,537	C3	4.00	8.00	10	0	1	1	0	0.017%	—	0.002%	0.002%	—	0.00%
3	21,662	C3	3.60	8.00	34	1	3	4	0	0.157%	0.005%	0.014%	0.018%	—	0.00%
4	6,785	C3	3.50	7.60	4	0	0	0	0	0.059%	—	—	—	—	—
5	18,393	C3	3.60	8.00	9	0	2	2	1	0.049%	—	0.011%	0.011%	1 : 18,393	50.00%
6	9,988	C3	3.60	8.00	1	0	0	0	0	0.010%	—	—	—	—	—
7	14,110	C3	3.60	8.00	6	—	—	0	—	0.043%	—	—	—	—	—
8	15,661	C3	3.60	8.00	12	7	0	7	2	0.077%	0.045%	—	0.0447%	1 : 7,831	28.57%
9	15,038	C3	4.00	—	4	0	0	0	0	0.027%	—	—	—	—	—
10	15,369	C3	3.60	8.00	5	0	0	0	0	0.033%	—	—	—	—	—
11	33,562	C3	3.60	8.00	2	0	1	1	1	0.006%	—	0.003%	0.003%	1 : 33,562	100.00%
12	13,801	C3	3.60	8.00	8	0	1	1	0	0.058%	—	0.007%	0.007%	—	0.00%
13	95,832	C3	3.60	8.00	25	2	3	5	2	0.026%	0.002%	0.003%	0.005%	1 : 47,916	40.00%
14	42,573	C3	4.00	8.00	26	1	—	1	—	0.061%	0.002%	—	0.002%	—	0.00%
16	24,488	C3	4.00	8.00	18	—	—	0	—	0.074%	—	—	—	—	—
17	65,106	C3	3.50	8.00	46	0	5	5	—	0.071%	—	0.008%	0.008%	—	0.00%
18	43,919	C3	3.50	—	—	1	2	3	1	—	0.002%	0.005%	0.007%	1 : 43,919	33.33%
19	42,358	C3	3.60	8.00	41	1	2	3	1	0.097%	0.002%	0.005%	0.007%	1 : 42,358	33.33%
20	14,058	C3	3.50	—	4	0	1	1	1	0.028%	—	0.007%	0.007%	1 : 14,058	100.00%
21	11,372	C3	3.80	8.00	7	0	1	1	1	0.062%	—	0.009%	0.009%	1 : 11,372	100.00%
22	7,270	C3	3.50	8.00	2	—	—	0	—	0.028%	—	—	—	—	—
23	15,864	C3	4.20	8.00	26	0	0	0	0	0.1639%	—	—	—	—	—
24	49,476	C3	3.60	8.00	21	1	0	1	—	0.042%	0.002%	—	0.002%	—	0.00%
25	7,533	C3	3.90	8.00	3	0	0	0	0	0.040%	—	—	—	—	—
26	43,346	C3	3.60	8.00	27	1	2	3	1	0.062%	0.002%	0.005%	0.007%	1 : 43,346	33.33%
27	9,457	C3	3.60	8.00	8	0	1	1	1	0.085%	—	0.011%	0.011%	1 : 9,457	100.00%
28	20,041	C3	3.60	8.00	5	0	0	0	0	0.025%	—	—	—	—	—
29	26,450	C3	3.60	8.00	5	1	1	2	0	0.019%	0.004%	0.004%	0.008%	—	0.00%
30	11,072	C3	3.50	8.00	3	0	0	0	0	0.027%	—	—	—	—	—
31	27,752	C3	3.60	8.00	30	0	2	2	—	0.108%	—	0.007%	0.0072%	—	0.00%
32	5,134	C3	4.00	8.00	9	0	1	1	0	0.175%	—	0.019%	0.019%	—	0.00%
33	13,684	C3	4.00	10.00	2	0	0	0	0	0.015%	—	—	—	—	—
34	20,794	C3	3.60	8.00	2	0	0	0	—	0.010%	—	—	—	—	—
36	14,517	C3	3.60	8.00	5	1	0	1	0	0.034%	0.007%	—	0.007%	—	0.00%
37	8,794	C3	3.60	—	15	0	0	0	0	0.171%	—	—	—	—	—
38	5,772	C3	3.60	7.50	—	—	—	0	—	—	—	—	—	—	—
全体	916,724	C3	3.69	8.03	480	19	31	50	12	0.052%	0.002%	0.003%	0.005%	1 : 76,394	24.00%
										max	0.175%	0.045%	0.019%	0.045%	100.00%
										min	0.006%	0.002%	0.002%	0.002%	0.00%

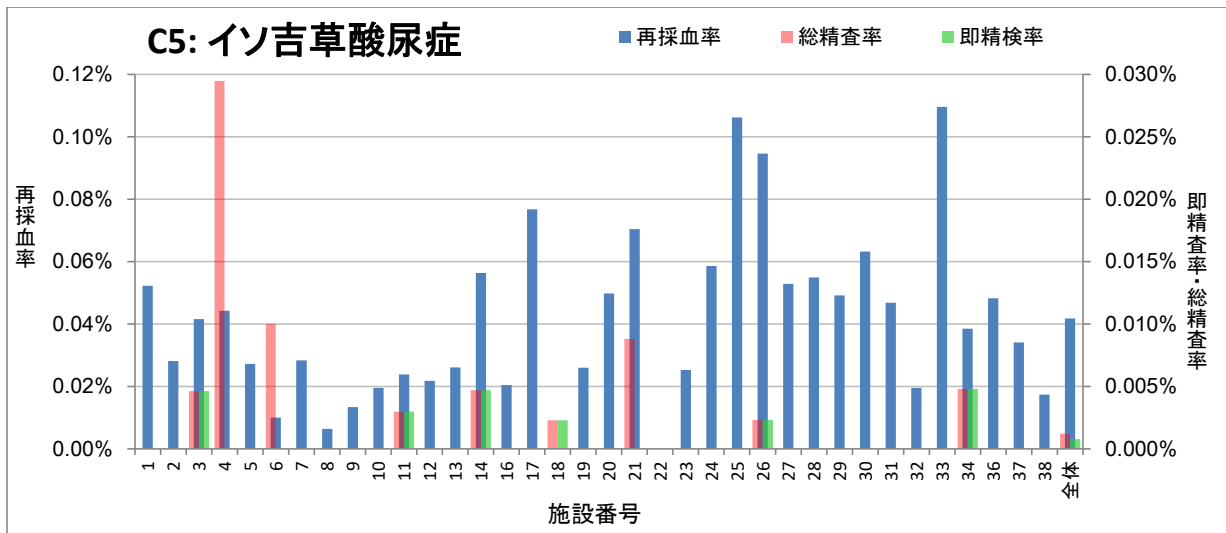


施設 No	検体数	項目	カットオフ値		再採 血数	即精 検数	再採血後 精検数	総精 検数	死 亡 患 者 数	再採血率	即精検率	再採血後 精検率	総精査率	発見頻度	陽性適中率 (PPV)
			初回 検査	即精査											
1	59,384	C5	1.00	5.00	31	0	0	0	0	0.052%	—	—	—	—	—
2	60,537	C5	1.00	5.00	17	0	0	0	0	0.028%	—	—	—	—	—
3	21,662	C5	1.00	4.00	9	1	0	1	0	0.042%	0.005%	—	0.005%	—	0.00%
4	6,785	C5	1.00	5.00	3	0	2	2	0	0.044%	—	0.029%	0.029%	—	0.00%
5	18,393	C5	1.00	—	5	0	0	0	0	0.027%	—	—	—	—	—
6	9,988	C5	1.00	5.00	1	—	1	1	0	0.010%	—	0.010%	0.010%	—	0.00%
7	14,110	C5	1.00	5.00	4	—	—	0	—	0.028%	—	—	—	—	—
8	15,661	C5	1.00	5.00	1	0	0	0	0	0.006%	—	—	—	—	—
9	15,038	C5	1.00	2.00	2	0	0	0	0	0.013%	—	—	—	—	—
10	15,369	C5	1.00	5.00	3	0	0	0	0	0.020%	—	—	—	—	—
11	33,562	C5	1.00	5.00	8	1	0	1	0	0.024%	0.003%	—	0.003%	—	0.00%
12	13,801	C5	1.00	5.00	3	0	0	0	0	0.022%	—	—	—	—	—
13	95,832	C5	1.00	5.00	25	0	0	0	0	0.026%	—	—	—	—	—
14	42,573	C5	1.00	5.00	24	2	—	2	—	0.056%	0.005%	—	0.005%	—	0.00%
16	24,488	C5	1.00	5.00	5	—	—	0	—	0.020%	—	—	—	—	—
17	65,106	C5	1.00	5.00	50	0	0	0	—	0.077%	—	—	—	—	—
18	43,919	C5	1.00	—	—	1	—	1	—	—	0.002%	—	0.002%	—	0.00%
19	42,358	C5	1.00	5.00	11	—	—	0	—	0.026%	—	—	—	—	—
20	14,058	C5	1.00	—	7	0	0	0	0	0.050%	—	—	—	—	—
21	11,372	C5	0.80	5.00	8	0	1	1	0	0.070%	—	0.009%	0.009%	—	0.00%
22	7,270	C5	1.00	5.00	—	—	—	0	—	—	—	—	—	—	—
23	15,864	C5	1.00	5.00	4	0	0	0	0	0.025%	—	—	—	—	—
24	49,476	C5	1.00	5.00	29	0	0	0	—	0.059%	—	—	—	—	—
25	7,533	C5	1.00	5.00	8	0	0	0	0	0.106%	—	—	—	—	—
26	43,346	C5	1.00	5.00	41	1	—	1	—	0.095%	0.002%	—	0.002%	—	0.00%
27	9,457	C5	0.90	5.00	5	0	0	0	0	0.053%	—	—	—	—	—
28	20,041	C5	1.00	5.00	11	0	0	0	0	0.055%	—	—	—	—	—
29	26,450	C5	1.00	5.00	13	0	0	0	0	0.049%	—	—	—	—	—
30	11,072	C5	1.00	5.00	7	0	0	0	0	0.063%	—	—	—	—	—
31	27,752	C5	1.00	5.00	13	0	0	0	—	0.047%	—	—	—	—	—
32	5,134	C5	1.00	5.00	1	0	0	0	0	0.019%	—	—	—	—	—
33	13,684	C5	1.00	5.00	15	0	0	0	0	0.110%	—	—	—	—	—
34	20,794	C5	1.00	5.00	8	1	0	1	—	0.038%	0.005%	—	0.005%	—	0.00%
36	14,517	C5	1.00	5.00	7	0	0	0	0	0.048%	—	—	—	—	—
37	8,794	C5	1.00	—	3	0	0	0	0	0.034%	—	—	—	—	—
38	5,772	C5	1.00	3.60	1	—	—	0	—	0.017%	—	—	—	—	—
全体	916,724	C5	0.99	4.83	383	7	4	11	0	0.042%	0.001%	0.000%	0.001%	—	0.00%
										max	0.110%	0.005%	0.029%	0.029%	0.00%
										min	0.006%	0.002%	0.009%	0.002%	0.00%

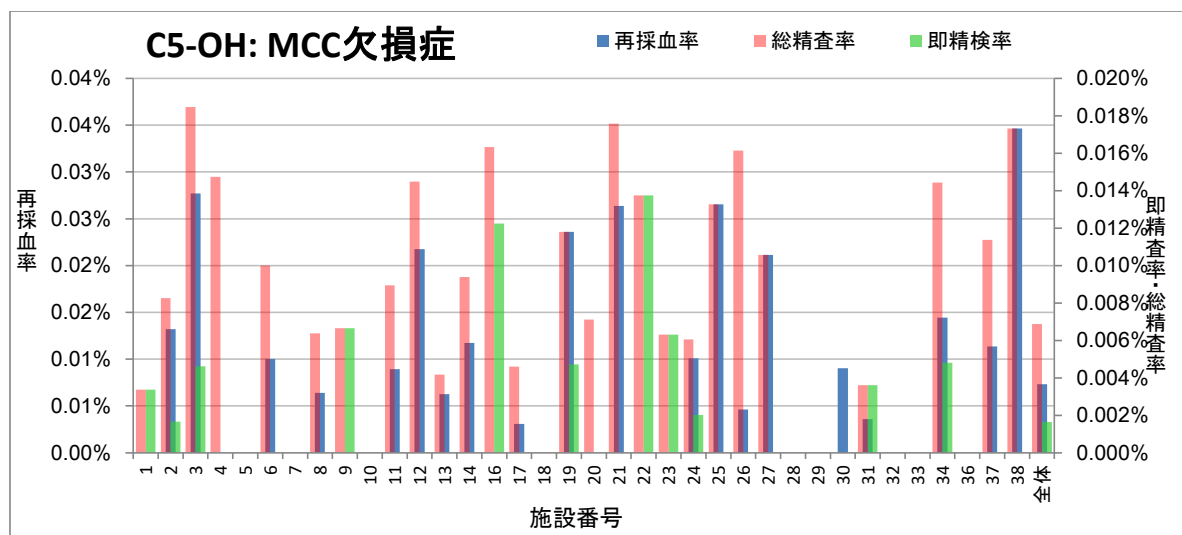


施設 No	検体数	項目	カットオフ値		再採 血数	即精 検数	再採血後 精検数	総精 検数	死 患者 数	再採血率	即精検率	再採血後 精検率	総精査率	発見頻度	陽性適中率 (PPV)
			初回 検査	即精査											
1	59,384	C5-OH	1.00	2.00	0	2	0	2	1	0.003%	0.003%	0.003%	0.003%	1:59,384	90.00%
2	60,537	C5-OH	1.00	2.00	8	1	4	5	1	0.013%	0.002%	0.007%	0.008%	1:60,537	20.00%
3	21,662	C5-OH	1.00	2.00	6	1	3	4	0	0.028%	0.005%	0.014%	0.018%	-	0.00%
4	6,785	C5-OH	1.00	2.00	0	0	1	1	0	-	-	0.015%	0.015%	-	0.00%
5	18,393	C5-OH	1.00	-	0	0	0	0	-	-	-	-	-	-	-
6	9,988	C5-OH	1.00	2.00	1	0	1	1	0	0.010%	-	0.010%	0.010%	-	0.00%
7	14,110	C5-OH	1.00	2.00	-	-	-	0	-	-	-	-	-	-	-
8	15,661	C5-OH	1.00	2.00	1	0	1	1	0	0.006%	-	0.006%	0.006%	-	0.00%
9	15,038	C5-OH	1.00	-	0	1	0	1	1	-	0.007%	-	0.007%	1:15,038	100.00%
10	15,369	C5-OH	1.00	2.00	0	0	0	0	0	-	-	-	-	-	-
11	33,562	C5-OH	1.00	2.00	3	0	3	3	0	0.009%	-	0.009%	0.009%	-	0.00%
12	13,801	C5-OH	1.00	2.00	3	0	2	2	0	0.022%	-	0.014%	0.014%	-	0.00%
13	95,832	C5-OH	1.00	2.00	6	0	4	4	1	0.006%	-	0.004%	0.004%	1:95,832	25.00%
14	42,573	C5-OH	1.00	2.00	5	-	4	4	-	0.012%	-	0.009%	0.009%	-	0.00%
16	24,488	C5-OH	1.00	2.00	-	3	1	4	-	-	0.012%	0.004%	0.016%	-	0.00%
17	65,106	C5-OH	0.60	2.00	2	0	3	3	-	0.003%	-	0.005%	0.005%	-	0.00%
18	43,919	C5-OH	1.00	-	-	-	-	0	-	-	-	-	-	-	-
19	42,358	C5-OH	1.00	2.00	10	2	3	5	1	0.024%	0.005%	0.007%	0.012%	1:42,358	20.00%
20	14,058	C5-OH	1.00	-	0	0	1	1	0	-	-	0.007%	0.007%	-	0.00%
21	11,372	C5-OH	0.80	2.00	3	0	2	2	0	0.026%	-	0.018%	0.018%	-	0.00%
22	7,270	C5-OH	1.00	2.00	-	1	-	1	1	-	0.014%	-	0.014%	1:7,270	100.00%
23	15,864	C5-OH	1.00	2.00	0	1	0	1	0	-	0.006%	-	0.006%	-	0.00%
24	49,476	C5-OH	1.00	2.00	5	1	2	3	-	0.010%	0.002%	0.004%	0.006%	-	0.00%
25	7,533	C5-OH	1.00	2.00	2	0	1	1	0	0.027%	-	0.013%	0.013%	-	0.00%
26	43,346	C5-OH	1.00	2.00	2	-	7	7	-	0.005%	-	0.016%	0.016%	-	0.00%
27	9,457	C5-OH	0.90	2.00	2	0	1	1	0	0.021%	-	0.011%	0.011%	-	0.00%
28	20,041	C5-OH	1.00	2.00	0	0	0	0	0	-	-	-	-	-	-
29	26,450	C5-OH	1.00	2.00	0	0	0	0	0	-	-	-	-	-	-
30	11,072	C5-OH	1.00	2.00	1	0	0	0	0	0.009%	-	-	-	-	-
31	27,752	C5-OH	1.00	2.00	1	1	0	1	-	0.004%	0.004%	-	0.004%	-	0.00%
32	5,134	C5-OH	1.40	2.00	0	0	0	0	0	-	-	-	-	-	-
33	13,684	C5-OH	0.90	2.00	0	0	0	0	0	-	-	-	-	-	-
34	20,794	C5-OH	1.00	2.00	3	1	2	3	-	0.014%	0.005%	0.010%	0.014%	-	0.00%
36	14,517	C5-OH	1.00	2.00	0	0	0	0	0	-	-	-	-	-	-
37	8,794	C5-OH	1.00	-	1	0	1	1	0	0.011%	-	0.011%	0.011%	-	0.00%
38	5,772	C5-OH	1.00	1.50	2	-	1	1	0	0.035%	-	0.017%	0.017%	-	0.00%
全体	916,724	C5-OH	0.99	1.98	67	15	48	63	6	0.01%	0.002%	0.005%	0.007%	1:152,787	9.52%
										max	0.035%	0.014%	0.018%		100.00%
										min	0.003%	0.002%	0.004%		0.00%

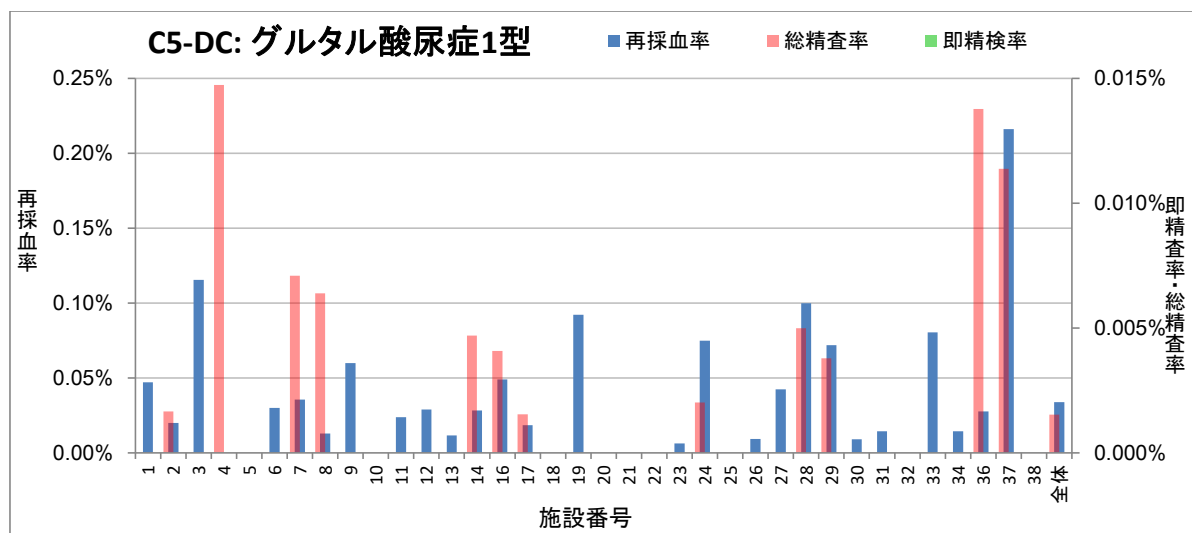


施設 No	検体数	項目	カットオフ値		再採 血数	即精 検数	再採血後 精検数	総精 検数	発見 患者 数	再採血率	即精検率	再採血後 精検率	総精査率	発見頻度	陽性適中率 (PPV)
			初回 検査	即精査											
1	59,384	C5-DC	0.30		28	0	0	1	0	0.047%	—	—	—	—	—
2	60,537	C5-DC	0.30		12	0	1	1	0	0.020%	—	0.002%	0.002%	—	0.00%
3	21,662	C5-DC	0.35		25	0	0	0	0	0.115%	—	—	—	—	—
4	6,785	C5-DC	0.31		0	0	1	1	0	—	—	0.015%	0.015%	—	0.00%
5	18,393	C5-DC	0.35		0	0	0	0	0	—	—	—	—	—	—
6	9,988	C5-DC	0.23		3	0	0	0	0	0.030%	—	—	—	—	—
7	14,110	C5-DC	0.25		5	0	1	1	0	0.035%	—	0.007%	0.007%	—	0.00%
8	15,661	C5-DC	0.30		2	0	1	1	0	0.013%	—	0.006%	0.006%	—	0.00%
9	15,038	C5-DC	0.35※1	0.50	9	0	0	0	0	0.060%	—	—	—	—	—
10	15,369	C5-DC	0.25		0	0	0	0	0	—	—	—	—	—	—
11	33,562	C5-DC	0.25		8	0	0	0	0	0.024%	—	—	—	—	—
12	13,801	C5-DC	0.25		4	0	0	0	0	0.029%	—	—	—	—	—
13	95,832	C5-DC	0.25	0.70	11	0	0	0	0	0.011%	—	—	—	—	—
14	42,573	C5-DC	0.35		12	0	2	2	0	0.028%	—	0.005%	0.005%	—	0.00%
16	24,488	C5-DC	0.27		12	0	1	1	0	0.049%	—	0.004%	0.004%	—	0.00%
17	65,106	C5-DC	0.25		12	0	1	1	0	0.018%	—	0.002%	0.002%	—	0.00%
18	43,919	C5-DC	0.30		—	—	—	0	—	—	—	—	—	—	—
19	42,358	C5-DC	0.25		39	0	0	0	0	0.092%	—	—	—	—	—
20	14,058	C5-DC	0.30		0	0	0	0	0	—	—	—	—	—	—
21	11,372	C5-DC	0.30		0	0	0	0	0	—	—	—	—	—	—
22	7,270	C5-DC	0.29		—	—	—	—	—	—	—	—	—	—	—
23	15,864	C5-DC	0.25		1	0	0	0	0	0.006%	—	—	—	—	—
24	49,476	C5-DC	0.25		37	0	1	1	0	0.075%	—	0.002%	0.002%	—	0.00%
25	7,533	C5-DC	0.35		0	0	0	0	0	—	—	—	—	—	—
26	43,346	C5-DC	0.29		4	0	—	—	0	0.009%	—	—	—	—	—
27	9,457	C5-DC	0.20		4	0	0	0	0	0.042%	—	—	—	—	—
28	20,041	C5-DC	0.20		20	0	1	1	0	0.100%	—	0.005%	0.005%	—	0.00%
29	26,450	C5-DC	0.25		19	0	1	1	1	0.072%	—	0.004%	0.004%	1:26,450	100.00%
30	11,072	C5-DC	0.30		1	0	0	0	0	0.009%	—	—	—	—	—
31	27,752	C5-DC	0.25		4	0	0	0	0	0.014%	—	—	—	—	—
32	5,134	C5-DC	0.25		0	0	0	0	0	—	—	—	—	—	—
33	13,684	C5-DC	0.35		11	0	0	0	0	0.080%	—	—	—	—	—
34	20,794	C5-DC	0.25		3	0	0	0	0	0.014%	—	—	—	—	—
36	14,517	C5-DC	0.25		4	0	2	2	0	0.028%	—	0.014%	0.014%	—	0.00%
37	8,794	C5-DC	0.20		19	0	1	1	0	0.216%	—	0.011%	0.011%	—	0.00%
38	5,772	C5-DC	0.35		—	—	—	—	—	—	—	—	—	—	—
全体	916,724	C5-DC	0.28	0.60	309	0	14	14	1	0.033%	—	0.002%	0.002%	1:916,724	7.14%
※1 2018年5月31日までは0.25μM										max	0.216%	0.000%	0.015%	0.015%	100.00%
										min	0.006%	0.000%	0.002%	0.002%	0.00%

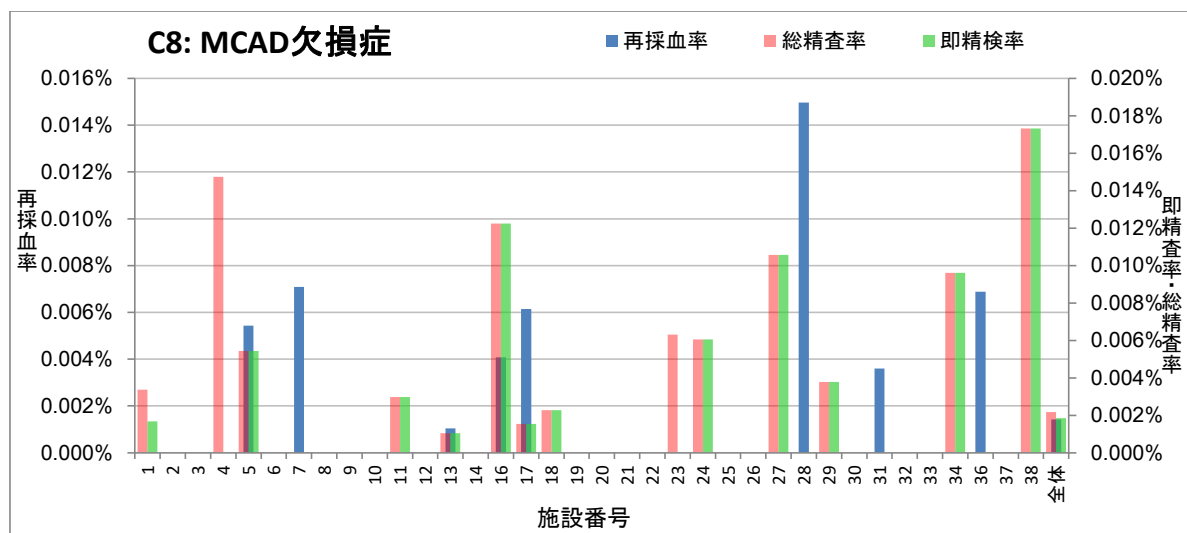


施設No	検体数	項目	カットオフ値		再採血数	即精検数	再採血後精検数	総精検数	死因患者数	再採血率	即精検率	再採血後精検率	総精査率	発見頻度	陽性適中率 (PPV)
			初回検査	即精査											
1	59,384	C8	0.30	0.50	0	1	1	2	0	—	0.002%	0.002%	0.003%	—	0.00%
2	60,537	C8	0.30	0.60	0	0	0	0	0	—	—	—	—	—	—
3	21,662	C8	0.30	0.30	0	0	0	0	0	—	—	—	—	—	—
4	6,785	C8	0.28	0.74	0	0	1	1	0	—	—	0.015%	0.015%	—	0.00%
5	18,393	C8	0.30	0.60	1	1	0	1	0	0.005%	0.005%	—	0.005%	—	0.00%
6	9,988	C8	—	0.23	0	0	0	0	0	—	—	—	—	—	—
7	14,110	C8	0.30	0.80	1	—	—	0	0	0.007%	—	—	—	—	—
8	15,661	C8	0.30	0.60	0	0	0	0	0	—	—	—	—	—	—
9	15,038	C8	0.30	0.50	0	0	0	0	0	—	—	—	—	—	—
10	15,369	C8	0.30	0.60	0	0	0	0	0	—	—	—	—	—	—
11	33,562	C8	—	0.30	0	1	0	1	0	—	0.003%	—	0.003%	—	0.00%
12	13,801	C8	—	0.30	—	0	—	0	0	—	—	—	—	—	—
13	95,832	C8	0.30	0.60	1	1	0	1	0	0.001%	0.001%	—	0.001%	—	0.00%
14	42,573	C8	0.30	0.30	—	—	—	0	—	—	—	—	—	—	—
16	24,488	C8	0.30	0.50	1	3	—	3	—	0.004%	0.012%	—	0.012%	—	0.00%
17	65,106	C8	0.30	0.60	4	1	0	1	0	0.006%	0.002%	—	0.002%	—	0.00%
18	43,919	C8	—	0.30	—	1	—	1	—	—	0.002%	—	0.002%	—	0.00%
19	42,358	C8	0.30	0.50	0	—	—	0	—	—	—	—	—	—	—
20	14,058	C8	0.30	—	0	0	0	0	0	—	—	—	—	—	—
21	11,372	C8	0.27	0.50	0	0	0	0	0	—	—	—	—	—	—
22	7,270	C8	0.30	0.50	—	—	—	0	—	—	—	—	—	—	—
23	15,864	C8	0.30	0.60	0	0	1	1	0	—	—	0.006%	0.006%	—	0.00%
24	49,476	C8	0.30	—	0	3	0	3	—	—	0.006%	—	0.006%	—	0.00%
25	7,533	C8	0.28	0.28	0	0	0	0	0	—	—	—	—	—	—
26	43,346	C8	0.30	0.30	0	—	—	0	—	—	—	—	—	—	—
27	9,457	C8	0.30	0.60	0	1	0	1	1	—	0.011%	—	0.011%	1:9,457	100.00%
28	20,041	C8	0.30	—	3	0	0	0	0	0.015%	—	—	—	—	—
29	26,450	C8	0.30	0.30	0	1	0	1	0	—	0.004%	—	0.004%	—	0.00%
30	11,072	C8	0.27	0.50	0	0	0	0	0	—	—	—	—	—	—
31	27,752	C8	0.30	0.30	1	0	0	0	0	0.004%	—	—	—	—	—
32	5,134	C8	0.30	0.60	0	0	0	0	0	—	—	—	—	—	—
33	13,684	C8	0.25	0.60	0	0	0	0	0	—	—	—	—	—	—
34	20,794	C8	0.40	0.40	0	2	0	2	—	—	0.010%	—	0.010%	—	0.00%
36	14,517	C8	—	0.30	1	0	0	0	0	0.007%	—	—	—	—	—
37	8,794	C8	0.30	0.30	0	0	0	0	0	—	—	—	—	—	—
38	5,772	C8	0.30	0.60	—	1	—	1	1	—	0.017%	—	0.017%	1:5,772	100.00%
全体	916,724	C8	0.30	0.47	13	17	3	20	2	0.001%	0.002%	0.000%	0.002%	1:458,362	10.00%
										max	0.015%	0.017%	0.015%	0.017%	100.00%
										min	0.001%	0.001%	0.002%	0.001%	0.00%

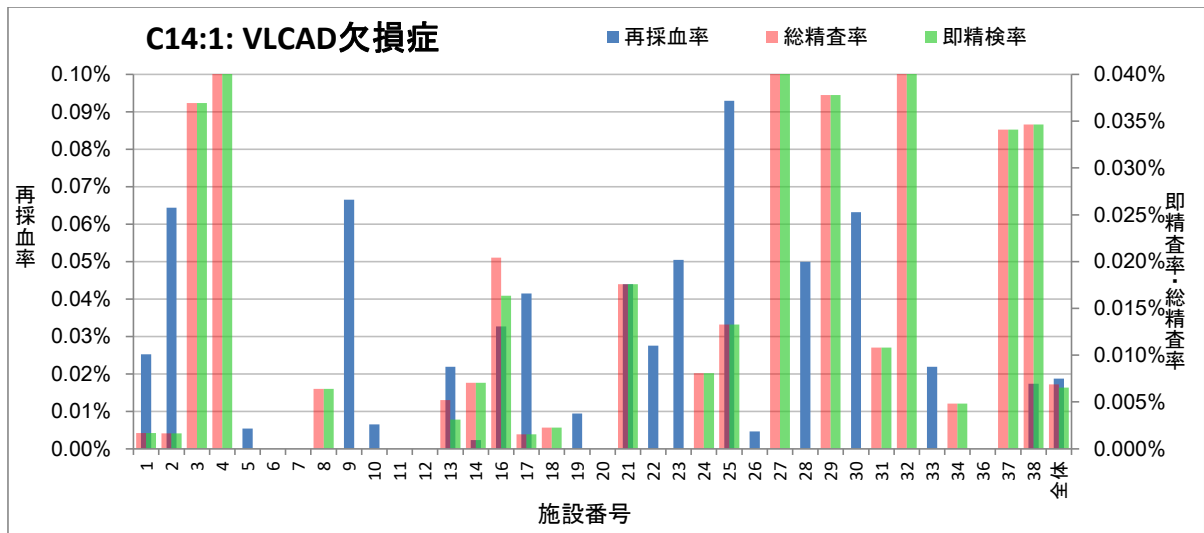


施設 No	検体数	項目	カットオフ値		再採 血数	即精 検数	再採血後 精検数	総精 検数	死 亡 患 者 数	再採血率	即精検率	再採血後 精検率	総精査率	発見頻度	陽性適中率 (PPV)
			初回 検査	即精査											
1	59,384	C14:1	0.35	1.00	15	1	0	1	0	0.025%	0.002%	—	0.002%	—	0.00%
2	60,537	C14:1	0.27	1.00	39	1	0	1	0	0.064%	0.002%	—	0.002%	—	0.00%
3	21,662	C14:1	0.30	0.30	0	8	0	8	0	—	0.037%	—	0.037%	—	0.00%
4	6,785	C14:1	0.21	0.21	0	3	0	3	0	—	0.044%	—	0.044%	—	0.00%
5	18,393	C14:1	0.40	—	1	0	0	0	0	0.005%	—	—	—	—	—
6	9,988	C14:1	—	0.28	0	0	0	0	0	—	—	—	—	—	—
7	14,110	C14:1	—	0.30	—	—	—	0	—	—	—	—	—	—	—
8	15,661	C14:1	0.40	—	0	1	0	1	1	—	0.006%	—	0.006%	1:15,661	100.00%
9	15,038	C14:1	0.30	1.00	10	0	0	0	0	0.066%	—	—	—	—	—
10	15,369	C14:1	0.30	1.00	1	0	0	0	0	0.007%	—	—	—	—	—
11	33,562	C14:1	0.40	1.00	0	0	0	0	0	—	—	—	—	—	—
12	13,801	C14:1	—	0.40	—	0	0	0	0	—	—	—	—	—	—
13	95,832	C14:1	0.40	0.40	21	3	2	5	3	0.022%	0.003%	0.002%	0.005%	1:31,944	60.00%
14	42,573	C14:1	0.40	0.40	1	3	—	3	1	0.002%	0.007%	—	0.007%	1:42,573	33.33%
16	24,488	C14:1	0.30	0.40	8	4	1	5	—	0.033%	0.016%	0.004%	0.020%	—	0.00%
17	65,106	C14:1	0.40	1.00	27	1	0	1	—	0.041%	0.002%	—	0.002%	—	0.00%
18	43,919	C14:1	—	0.40	—	1	—	1	—	—	0.002%	—	0.002%	—	0.00%
19	42,358	C14:1	0.40	1.00	4	—	—	0	—	0.009%	—	—	—	—	—
20	14,058	C14:1	0.40	—	0	0	0	0	0	—	—	—	—	—	—
21	11,372	C14:1	0.27	1.00	5	2	0	2	1	0.044%	0.018%	—	0.018%	1:11,372	50.00%
22	7,270	C14:1	0.27	1.00	2	—	—	0	—	0.028%	—	—	—	—	—
23	15,864	C14:1	0.30	1.00	8	0	0	0	0	0.050%	—	—	—	—	—
24	49,476	C14:1	0.40	—	0	4	0	4	—	—	0.008%	—	0.008%	—	0.00%
25	7,533	C14:1	0.30	0.30	7	1	0	1	0	0.093%	0.013%	—	0.013%	—	0.00%
26	43,346	C14:1	0.40	0.40	2	—	—	0	—	0.005%	—	—	—	—	—
27	9,457	C14:1	0.30	—	0	4	0	4	1	—	0.042%	—	0.042%	1:9,457	25.00%
28	20,041	C14:1	0.35	—	10	0	0	0	0	0.050%	—	—	—	—	—
29	26,450	C14:1	0.40	0.40	0	10	0	10	0	—	0.038%	—	0.038%	—	0.00%
30	11,072	C14:1	0.30	1.00	7	0	0	0	0	0.063%	—	—	—	—	—
31	27,752	C14:1	0.40	0.40	0	3	0	3	—	—	0.011%	—	0.011%	—	0.00%
32	5,134	C14:1	0.30	—	0	4	0	4	0	—	0.078%	—	0.078%	—	0.00%
33	13,684	C14:1	0.30	0.80	3	0	0	0	0	0.022%	—	—	—	—	—
34	20,794	C14:1	0.40	0.40	0	1	0	1	—	—	0.005%	—	0.005%	—	0.00%
36	14,517	C14:1	—	0.40	0	0	0	0	0	—	—	—	—	—	—
37	8,794	C14:1	0.25	0.25	0	3	0	3	0	—	0.034%	—	0.034%	—	0.00%
38	5,772	C14:1	0.35	1.00	1	2	—	2	0	0.017%	0.035%	—	0.035%	—	0.00%
全体	916,724	C14:1	0.34	0.64	172	60	3	63	7	0.019%	0.007%	0.000%	0.007%	1:130,961	11.11%
										max	0.093%	0.078%	0.004%	0.078%	100.00%
										min	0.002%	0.002%	0.002%	0.002%	0.00%

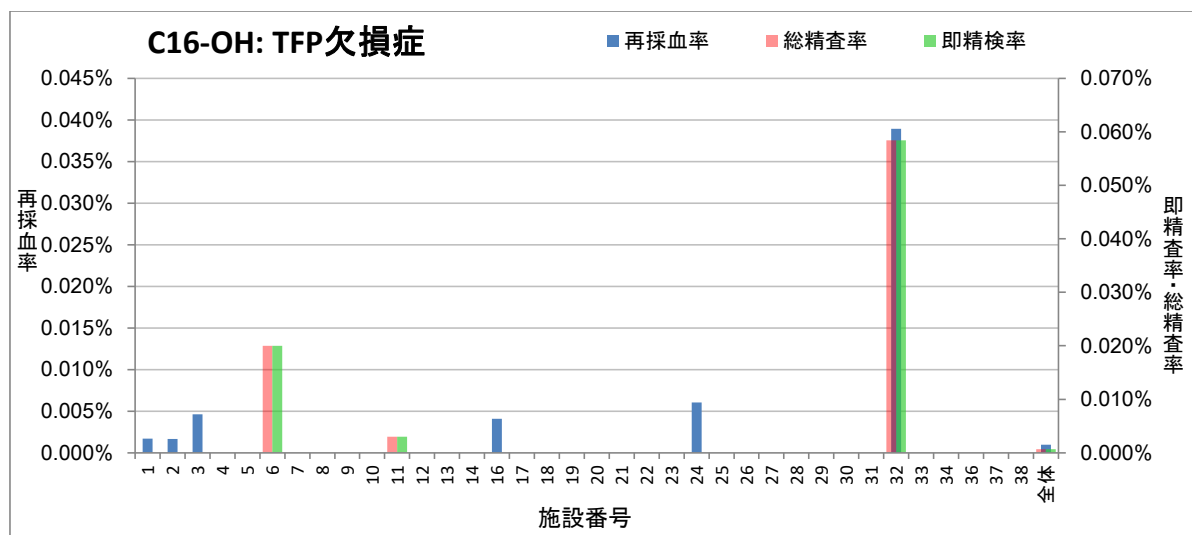

施設 No	検体数	項目	カットオフ値		再採 血数	即精 検数	再採血後 精検数	総精 検数	死 亡 患 者 数	再採血率	即精検率	再採血後 精検率	総精査率	発見頻度	陽性適中率 (PPV)
			初回 検査	即精査											
1	59,384	C16-OH	0.05		1	0	0	0	0	0.002%	-	-	-	-	-
2	60,537	C16-OH	0.05		1	0	0	0	0	0.002%	-	-	-	-	-
3	21,662	C16-OH	0.05	0.05	1	0	0	0	0	0.005%	-	-	-	-	-
4	6,785	C16-OH	0.08	0.08	0	0	0	0	0	-	-	-	-	-	-
5	18,393	C16-OH	0.10		0	0	0	0	-	-	-	-	-	-	-
6	9,988	C16-OH		0.05	0	2	0	2	0	-	0.020%	-	0.020%	-	0.00%
7	14,110	C16-OH	0.10					0	-	-	-	-	-	-	-
8	15,661	C16-OH	0.05		0	0	0	0	0	-	-	-	-	-	-
9	15,038	C16-OH	0.10		0	0	0	0	0	-	-	-	-	-	-
10	15,369	C16-OH	0.08		0	0	0	0	0	-	-	-	-	-	-
11	33,562	C16-OH		0.10	0	1	0	1	0	-	0.003%	-	0.003%	-	0.00%
12	13,801	C16-OH		0.10		0		0	0	-	-	-	-	-	-
13	95,832	C16-OH	0.05		0	0	0	0	0	-	-	-	-	-	-
14	42,573	C16-OH	0.10	0.10				0	-	-	-	-	-	-	-
16	24,488	C16-OH	0.05		1			0	-	0.004%	-	-	-	-	-
17	65,106	C16-OH	0.05		0	0	0	0	-	-	-	-	-	-	-
18	43,919	C16-OH		0.04	-			0	-	-	-	-	-	-	-
19	42,358	C16-OH	0.05		0			0	-	-	-	-	-	-	-
20	14,058	C16-OH	0.05		0	0	0	0	0	-	-	-	-	-	-
21	11,372	C16-OH	0.05		0	0	0	0	0	-	-	-	-	-	-
22	7,270	C16-OH	0.05					0	-	-	-	-	-	-	-
23	15,864	C16-OH	0.08		0	0	0	0	0	-	-	-	-	-	-
24	49,476	C16-OH	0.04		3	0	0	0	-	0.006%	-	-	-	-	-
25	7,533	C16-OH	0.10	0.10	0	0	0	0	0	-	-	-	-	-	-
26	43,346	C16-OH	0.05	0.05	0			0	-	-	-	-	-	-	-
27	9,457	C16-OH	0.06		0	0	0	0	0	-	-	-	-	-	-
28	20,041	C16-OH	0.10		0	0	0	0	0	-	-	-	-	-	-
29	26,450	C16-OH	0.10	0.10	0	0	0	0	0	-	-	-	-	-	-
30	11,072	C16-OH	0.05		0	0	0	0	0	-	-	-	-	-	-
31	27,752	C16-OH	0.07	0.07	0	0	0	0	-	-	-	-	-	-	-
32	5,134	C16-OH	0.08		2	3	0	3	0	0.039%	0.058%	-	0.058%	-	0.00%
33	13,684	C16-OH	0.05		0	0	0	0	0	-	-	-	-	-	-
34	20,794	C16-OH	0.06		0	0	0	0	-	-	-	-	-	-	-
36	14,517	C16-OH		0.10	0	0	0	0	0	-	-	-	-	-	-
37	8,794	C16-OH	0.08		0	0	0	0	0	-	-	-	-	-	-
38	5,772	C16-OH	0.08					0	-	-	-	-	-	-	-
全体	916,724	C16-OH	0.07	0.08	9	6	0	6	0	0.00%	0.001%	-	0.001%	-	0.00%
										max	0.039%	0.058%	0.000%	0.058%	0.00%
										min	0.002%	0.003%	0.000%	0.003%	0.00%

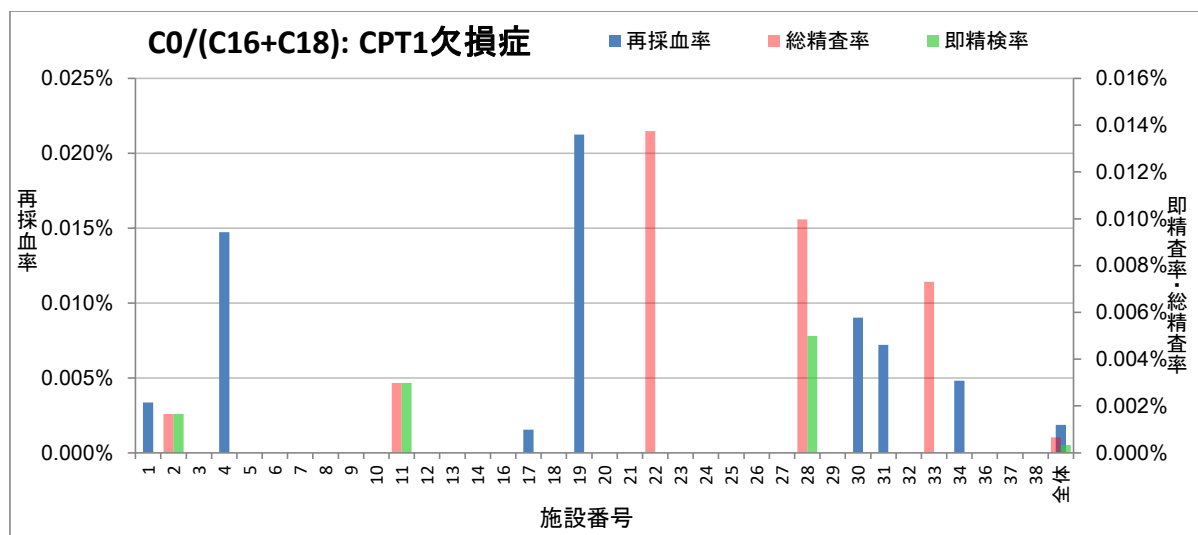

施設 No	検体数	項目	カットオフ値		再採 血数	即精 検数	再採血後 精検数	総精 検数	死 亡 患 者 数	再採血率	即精検率	再採血後 精検率	総精査率	発見頻度	陽性適中率 (PPV)
			初回 検査	即精査											
1	59,384	C0/(C16+C18)	90.00		2	0	0	0	0	0.003%	—	—	—	—	—
2	60,537	C0/(C16+C18)	100.00		0	1	0	1	0	—	0.002%	—	0.002%	—	0.00%
3	21,662	C0/(C16+C18)	80.00		0	0	0	0	0	—	—	—	—	—	—
4	6,785	C0/(C16+C18)	96.00		1	0	0	0	0	0.015%	—	—	—	—	—
5	18,393	C0/(C16+C18)	100.00		0	0	0	0	—	—	—	—	—	—	—
6	9,988	C0/(C16+C18)	80.00		0	0	0	0	—	—	—	—	—	—	—
7	14,110	C0/(C16+C18)	100.00					0	—	—	—	—	—	—	—
8	15,661	C0/(C16+C18)	100.00		0	0	0	0	—	—	—	—	—	—	—
9	15,038	C0/(C16+C18)	100.00		0	0	0	0	—	—	—	—	—	—	—
10	15,369	C0/(C16+C18)	40.00		0	0	0	0	—	—	—	—	—	—	—
11	33,562	C0/(C16+C18)		100.00	0	1	0	1	0	—	0.003%	—	0.003%	—	0.00%
12	13,801	C0/(C16+C18)		100.00		0		0	0	—	—	—	—	—	—
13	95,832	C0/(C16+C18)	100.00		0	0	0	0	—	—	—	—	—	—	—
14	42,573	C0/(C16+C18)	100.00	100.00				0	—	—	—	—	—	—	—
16	24,488	C0/(C16+C18)	80.00					0	—	—	—	—	—	—	—
17	65,106	C0/(C16+C18)	100.00		1	0	0	0	—	0.002%	—	—	—	—	—
18	43,919	C0/(C16+C18)		100.00	—			0	—	—	—	—	—	—	—
19	42,358	C0/(C16+C18)	70.00		9			0	—	0.021%	—	—	—	—	—
20	14,058	C0/(C16+C18)	100.00		0	0	0	0	—	—	—	—	—	—	—
21	11,372	C0/(C16+C18)	50.00		0	0	0	0	—	—	—	—	—	—	—
22	7,270	C0/(C16+C18)	60.00				1	1	—	—	—	0.014%	0.014%	—	0.00%
23	15,864	C0/(C16+C18)	100.00		0	0	0	0	—	—	—	—	—	—	—
24	49,476	C0/(C16+C18)	100.00		0	0	0	0	—	—	—	—	—	—	—
25	7,533	C0/(C16+C18)	75.00	75.00	0	0	0	0	—	—	—	—	—	—	—
26	43,346	C0/(C16+C18)	60.00		0			0	—	—	—	—	—	—	—
27	9,457	C0/(C16+C18)	80.00		0	0	0	0	—	—	—	—	—	—	—
28	20,041	C0/(C16+C18)	100.00		0	1	1	2	0	—	0.005%	0.005%	0.010%	—	0.00%
29	26,450	C0/(C16+C18)	100.00	100.00	0	0	0	0	—	—	—	—	—	—	—
30	11,072	C0/(C16+C18)	60.00		1	0	0	0	0	0.009%	—	—	—	—	—
31	27,752	C0/(C16+C18)	50.00		2	0	0	0	—	0.007%	—	—	—	—	—
32	5,134	C0/(C16+C18)	40.00		0	0	0	0	—	—	—	—	—	—	—
33	13,684	C0/(C16+C18)	80.00		0	0	1	1	—	—	—	0.007%	0.007%	—	0.00%
34	20,794	C0/(C16+C18)	100.00		1	0	0	0	—	0.005%	—	—	—	—	—
36	14,517	C0/(C16+C18)		100.00	0	0	0	0	—	—	—	—	—	—	—
37	8,794	C0/(C16+C18)	40.00		0	0	0	0	—	—	—	—	—	—	—
38	5,772	C0/(C16+C18)	100.00					0	—	—	—	—	—	—	—
全体	916,724	C0/(C16+C18)	82.22	96.43	17	3	3	6	0	0.00%	0.000%	0.000%	0.001%	—	0.00%
										max	0.021%	0.005%	0.014%	0.014%	0.00%
										min	0.002%	0.002%	0.005%	0.002%	0.00%

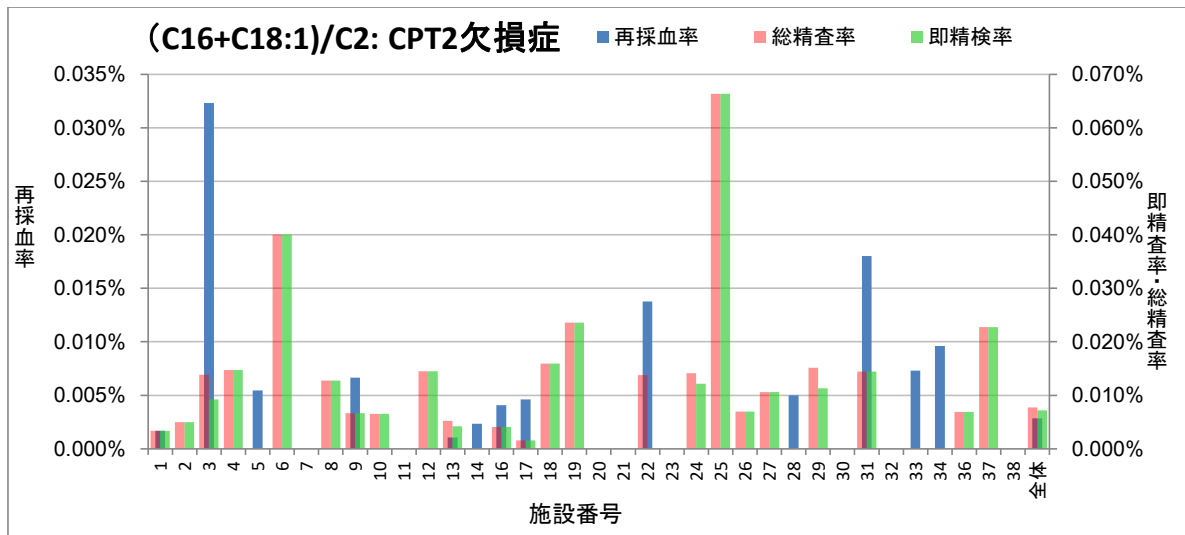

施設 No	検体数	項目	カットオフ値		再採 血数	即精 検数	再採血後 精検数	総精 検数	発 見 患 者 数	再採血率	即精検率	再採血後 精検率	総精査率	発見頻度	陽性適中率 (PPV)
			初回 検査	即精査											
1	59,384	(C16+C18:1)/C2		0.34	1	2	0	2	0	0.002%	0.003%	—	0.003%	—	0.00%
2	60,537	(C16+C18:1)/C2	0.65	0.65	0	3	0	3	1	—	0.005%	—	0.005%	1:60,537	33.33%
3	21,662	(C16+C18:1)/C2	0.38	0.38	7	2	1	3	0	0.032%	0.009%	0.005%	0.014%	—	0.00%
4	6,785	(C16+C18:1)/C2	0.37	0.37	0	1	0	1	0	—	0.015%	—	0.015%	—	0.00%
5	18,393	(C16+C18:1)/C2	0.45		1	0	0	0	—	0.005%	—	—	—	—	—
6	9,988	(C16+C18:1)/C2		0.39	0	4	0	4	0	—	0.040%	—	0.040%	—	0.00%
7	14,110	(C16+C18:1)/C2		0.40				0	—	—	—	—	—	—	—
8	15,661	(C16+C18:1)/C2	0.40		0	2	0	2	0	—	0.013%	—	0.013%	—	0.00%
9	15,038	(C16+C18:1)/C2	0.40		1	1	0	1	1	0.007%	0.007%	—	0.007%	1:15,038	100.00%
10	15,369	(C16+C18:1)/C2	0.42		0	1	0	1	0	—	0.007%	—	0.007%	—	0.00%
11	33,562	(C16+C18:1)/C2		0.40	0	0	0	0	0	—	—	—	—	—	—
12	13,801	(C16+C18:1)/C2		0.35		2		2	0	—	0.014%	—	0.014%	—	0.00%
13	95,832	(C16+C18:1)/C2	0.40		1	4	1	5	1	0.001%	0.004%	0.001%	0.005%	1:95,832	20.00%
14	42,573	(C16+C18:1)/C2	0.37	0.37	1			0	—	0.002%	—	—	—	—	—
16	24,488	(C16+C18:1)/C2		0.40	1	1		1	—	0.004%	0.004%	—	0.004%	—	0.00%
17	65,106	(C16+C18:1)/C2	0.36		3	1	0	1	—	0.005%	0.002%	—	0.002%	—	0.00%
18	43,919	(C16+C18:1)/C2		0.40	—	7		7	—	—	0.016%	—	0.016%	—	0.00%
19	42,358	(C16+C18:1)/C2		0.41	0	10		10	—	—	0.024%	—	0.024%	—	0.00%
20	14,058	(C16+C18:1)/C2	0.50		0	0	0	0	0	—	—	—	—	—	—
21	11,372	(C16+C18:1)/C2	0.40		0	0	0	0	0	—	—	—	—	—	—
22	7,270	(C16+C18:1)/C2	0.36		1		1	1	1	0.014%	—	0.014%	0.014%	1:7,270	100.00%
23	15,864	(C16+C18:1)/C2	0.57		0	0	0	0	0	—	—	—	—	—	—
24	49,476	(C16+C18:1)/C2	0.50		0	6	1	7	—	—	0.012%	0.002%	0.014%	—	0.00%
25	7,533	(C16+C18:1)/C2	0.37	0.37	0	5	0	5	0	—	0.066%	—	0.066%	—	0.00%
26	43,346	(C16+C18:1)/C2	0.43	0.43	0	3		3	—	—	0.007%	—	0.007%	—	0.00%
27	9,457	(C16+C18:1)/C2	0.50		0	1	0	1	0	—	0.011%	—	0.011%	—	0.00%
28	20,041	(C16+C18:1)/C2	0.45		1	0	0	0	0	0.005%	—	—	—	—	—
29	26,450	(C16+C18:1)/C2	0.32	0.32	0	3	1	4	0	—	0.011%	0.004%	0.015%	—	0.00%
30	11,072	(C16+C18:1)/C2		0.42	0	0	0	0	0	—	—	—	—	—	—
31	27,752	(C16+C18:1)/C2	0.44	0.44	5	4	0	4	—	0.018%	0.014%	—	0.014%	—	0.00%
32	5,134	(C16+C18:1)/C2	0.57		0	0	0	0	0	—	—	—	—	—	—
33	13,684	(C16+C18:1)/C2	0.44		1	0	0	0	0	0.007%	—	—	—	—	—
34	20,794	(C16+C18:1)/C2	0.39	0.39	2	0	0	0	—	0.010%	—	—	—	—	—
36	14,517	(C16+C18:1)/C2		0.54	0	1	0	1	0	—	0.007%	—	0.007%	—	0.00%
37	8,794	(C16+C18:1)/C2	0.50	0.50	0	2	0	2	0	—	0.023%	—	0.023%	—	0.00%
38	5,772	(C16+C18:1)/C2	0.40					0	—	—	—	—	—	—	—
全体	916,724	(C16+C18:1)/C2	0.44	0.41	26	66	5	71	4	0.00%	0.007%	0.001%	0.008%	1:229,181	5.63%
										max	0.032%	0.066%	0.014%		100.00%
										min	0.001%	0.002%	0.001%		0.00%